

SPECMONUP
Options 10, 11, 12, 21, 22, and 52
SPECMON Series Real-Time Spectrum Analyzers
Software Upgrades
Instructions

www.tektronix.com



071-3072-00

Tektronix

Copyright © Tektronix. All rights reserved. Licensed software products are owned by Tektronix or its subsidiaries or suppliers, and are protected by national copyright laws and international treaty provisions.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specifications and price change privileges reserved.

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

Contacting Tektronix

Tektronix, Inc.
14150 SW Karl Braun Drive
P.O. Box 500
Beaverton, OR 97077
USA

For product information, sales, service, and technical support:

- In North America, call 1-800-833-9200.
- Worldwide, visit www.tektronix.com to find contacts in your area.

Table of Contents

Kit description	1
Products	1
Kit parts list.....	1
Minimum tool and equipment list.....	1
Install option key	2
Attach labels.....	4
Verify instrument software version	4

Kit description

This kit describes the installation of the Option 10, 11, 12, 21, 22, and 52 Upgrades in SPECMON Series instruments.

The option you've ordered only requires that you enter a key code to activate your option.

For a list of available options, see the Tektronix Web site (www.tektronix.com) or your Tektronix representative.

Products

SPECMON3. All serial numbers

SPECMON6. All serial numbers

Kit parts list

Quantity	Part number	Description
1 ea	071-3072-XX	MANUAL, TECH: INSTALLATION
1 ea	N/A	SOFTWARE OPTION KEY AUTHORIZATION CERTIFICATE, UPGRADE KITS
1 ea	N/A	LABEL, MANUFACTURED; OPTION KEY UPGRADE LABEL 2.100 X 2.700, SAFETY CONTROLLED


Minimum tool and equipment list

Name	Description
Keyboard	Standard accessory provided with the instrument


Install option key

To activate your new option, you must enter a new option key.

1. Power on the instrument.
2. Select **Tools > Install Upgrades...** to start the upgrade installation process.
3. Click Continue from the Install Upgrades introduction screen.

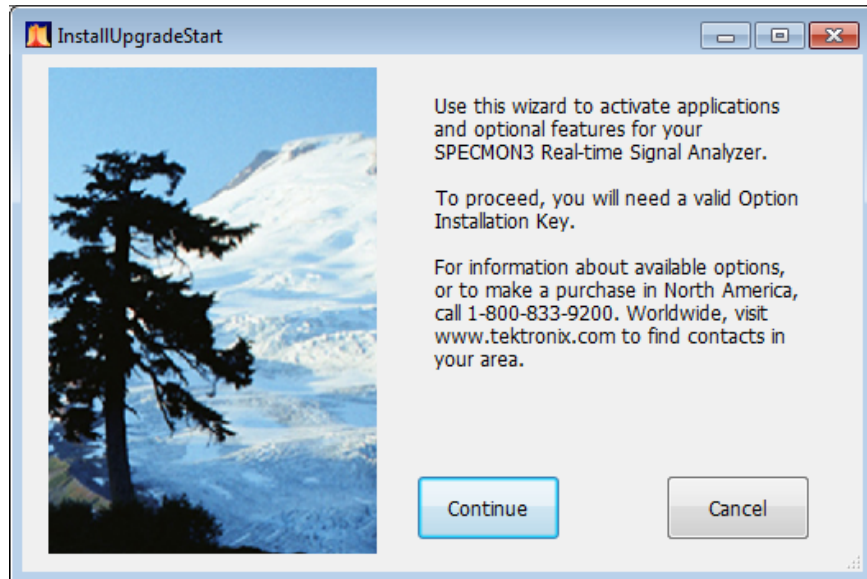

4. Enter the option key provided by Tektronix, and follow the on-screen instructions to install the option.

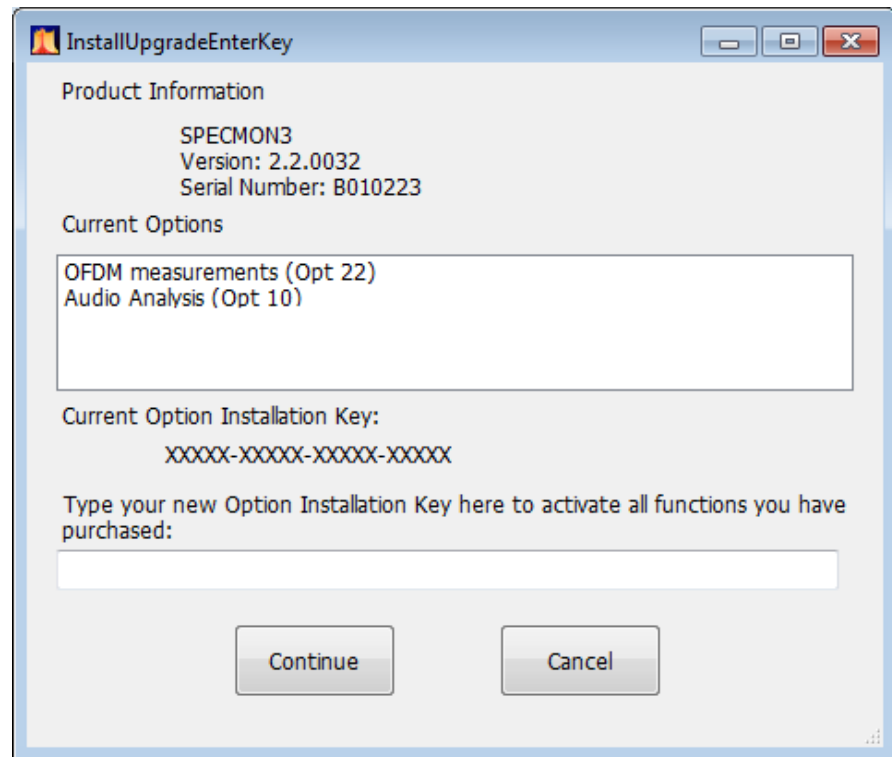

5. Power off the instrument, then power back on.
6. In the Help menu, select About Tektronix Real-Time Analyzer.
7. Verify the new option is listed.

Attach labels

Please attach all labels provided in this kit on the instrument's rear panel.

Attach the option key label

Place the new option key label over the existing label on the instrument rear panel.

NOTE. *This label is not included with all options.*

Attach the product/option label

Place the new product key label over the existing label on the instrument rear panel if this label is included with your option.

Verify instrument software version

Tektronix recommends to update to the latest available application software for your instrument.

1. Select **Help** > **About** to check the software version.
2. Use your Web browser to go to: www.tektronix.com/software.
3. Search for your instrument's model number and follow the link to the software.
4. If the installed software is older than that available, download the software.
5. Follow the instructions on the Web page to install the software.

■ End of Document ■