

Digital Power Management Analysis

5/6 Series B MSO Option 5-DPMBAS/5-DPM/6-DPM Application Datasheet



Most of today's electronic designs require different supply voltages to function properly. Some components within a given circuit require multiple voltage levels. Testing a product for its specification is a time consuming process; debugging is even more cumbersome process. Hence, power integrity has started playing a significant role and the companies are able to improve their time to market.

The Digital Power Management and Analysis (DPM) software option provides automated power rail measurements for the Power Integrity Analysis on the 5/6 Series B MSO. The solution enables simultaneous analysis of multiple power rails using power rail probes and sequencing of measurements using passive probes. The solution is designed with the user work flow in mind to help design engineers meet their time-to-market needs. It also generates an automated report that includes measurements, test results, and plot images.

The solution in combination with the Tektronix 5/6 Series B MSO and Tektronix Power Rail Probes helps engineers to measure and analyze Ripple, Transient characteristics, Power Supply Sequencing, Amplitude, Jitter, Eye, and timing diagrams and perform measurements repeatably, analyse results to increase accuracy. The multiple FlexChannel® inputs, SI/PI, and the next generation user interface of the 5/6 Series B MSO enables engineers to view the waveform (time-domain), a spectral view (frequency domain), or both simultaneously to efficiently debug and analyze the circuit design.

Salient Features of the software solution

- Test up to 7 rails simultaneously with automated measurements and configure each channel
- Allows you to identify the source of the ripple
- Analyze high frequency ripple overlaid on ripple for better design – Ripple on Ripple
- PSIJ measurement identifies the inter-dependency between high speed serial load and power rail noise
- Single click detection and set up of probes
- Auto-zero: User can deskew probes from menu for each channel


Customer applications

Power integrity analysis plays a critical role especially with highly-integrated system on chip and microprocessor designs in which multiple technologies interface together. It is important to look at each DC line to see if the power supplied is within the tolerance band of a target system or device. The typical applications can be found across industries that need power conversion and have multiple DC voltage levels in the circuit design. Some examples include:

- Mobiles, Computers, and Tablets
- Automotive
- Industrial
- Data center


Measurement overview

Two of the most important measurements while analyzing a Power Supply design are Ripple and Transient. However, when looking at the complex IC designs these days, there are a few other measurements like Power Sequencing, Jitter and Signal Integrity-Power Integrity (SI/PI) that have also become important.

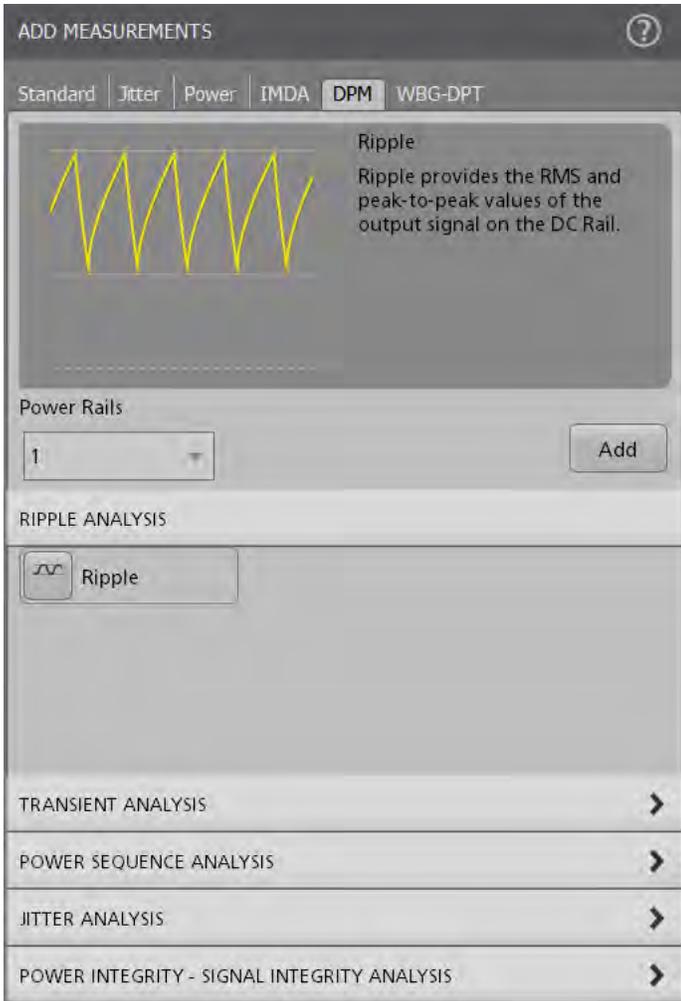


The Digital Power Management solution enables the analysis of multiple power rails simultaneously to reduce test times during design and validation. The 8-channel 5 Series B/6 Series B MSO can measure up to 7 power rails at once.

The solution also leverages the Spectrum View capability to perform Spectrum Analysis on the ripple. This helps the designers to identify the source of ripple and help to save a lot of time and effort on debugging.

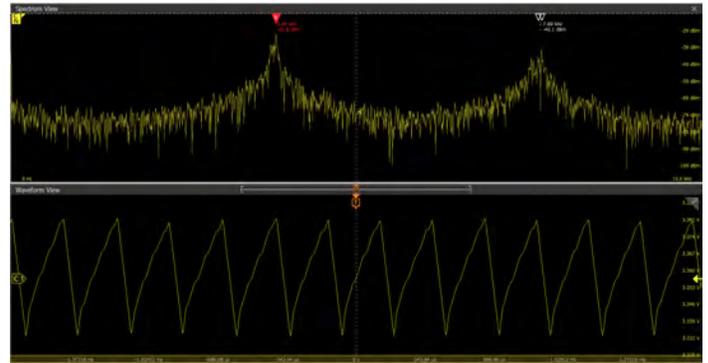

Analyze cycle-by-cycle by selecting a PWM clock (if available) and view peak-peak and RMS values for each ripple cycle. This gives statistics for all of the cycles within an acquisition. Bandwidth limit capability enables designers to analyze the ripple numbers at different bandwidths.

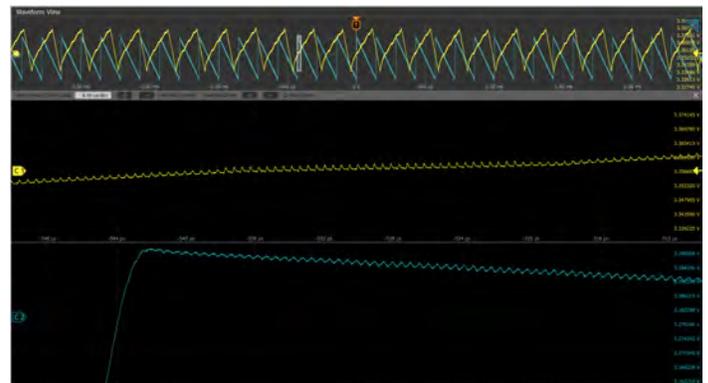

One of the unique features of the DPM solution is the ability to leverage the capabilities of the Power Rail probes to analyze additional high frequency noise overlaid on the ripple. This is typically known as Ripple-on-Ripple.


Power sequence analysis

Power sequence analysis enables power designers to ensure that the power rails reach the on or off states within the expected times.

Power sequence analysis runs simultaneously on up to seven power rails. Configure the eighth source as a reference input to measure the turn-on and turn-off time. This enables the designers to measure the power sequencing of their power rails and ensure they reach their turn-on and turn-off states within the required times. Automating these


Ripple analysis

In simple terms, Ripple is defined as the residual AC voltage on a constant DC component (offset). Typically, the ripple component is often small in magnitude relative to the DC component.

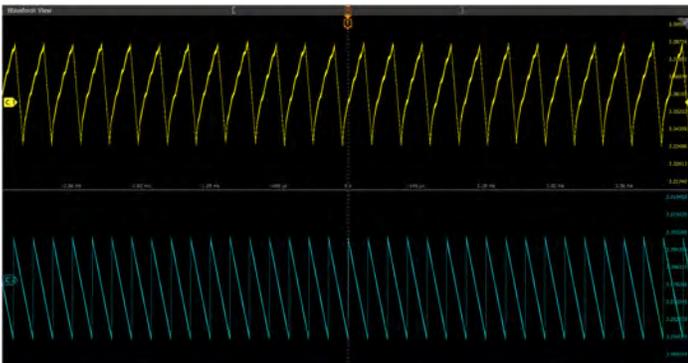

Designers should not confuse Ripple with the System noise. It is possible to see only the ripple by minimizing oscilloscope and probe noise when measuring DC power rails.

tests helps achieve consistent and accurate results under different load conditions.

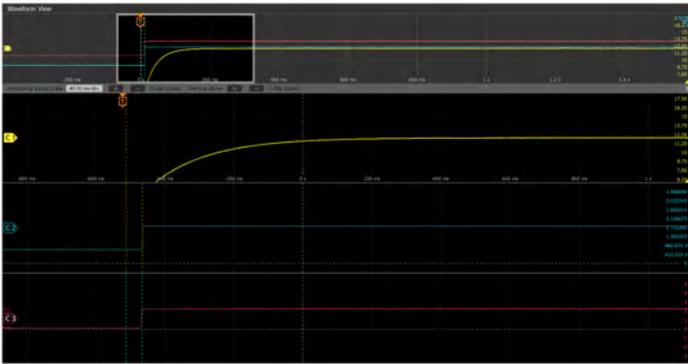


To set up the test, configure the nominal input and output voltages, trigger level, and wait time (duration). Pressing the Power Rail Preset button initiates an optimization process in which the software optimizes scale settings, record length, and sample rate for the best results. Turn-on and turn-off times are displayed in the results badge and indicated on the waveform with colors. Results are also available in a tabular format. Compare and validate the design for wait times by observing the results table for anomalies.

Transient analysis

A transient phenomenon in a system is caused by a change of the operating conditions or the system configuration. The importance of transient analysis is to identify the effects the disturbances have on the system performance or the failures they cause to power equipment.

Transient analysis typically includes overshoot and undershoot measurements. Just like Ripple, the application allows for simultaneous automated measurements with a few simple steps. A reference voltage is entered for each power rail before initiating the test. The overshoot measurement gives the difference between the maximum voltage and the reference voltage. The undershoot measurement gives the difference between the minimum voltage and the reference voltage.

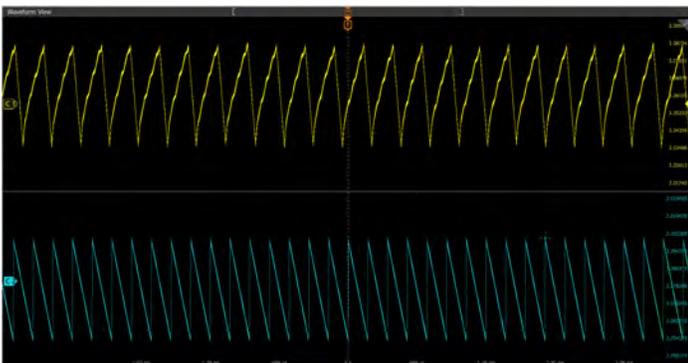


Perform this measurement for a single cycle within an acquisition or over every cycle within an acquisition (Cycle Mode). Synchronize cycles based on a power rail signal or another signal in the system. Cycle-by-cycle measurements are analyzed using statistics, histograms, or

plots. Bandwidth limit capability enables designers to analyze the ripple numbers at different bandwidths.

Jitter analysis

Jitter measurements help to validate the jitter tolerances on the high-speed side, which uses the DPM outputs to power-on their loads. The common noise sources are crosstalk from data signals, coupling from clocks and power supply switching noise (and harmonics) and SSN (Simultaneous Switching Noise). The DPM multi-rail outputs power on different loads such as FPGA, system/CPU clocks, DDR memories, transceivers, etc. Both, Power Integrity (PI) and Signal Integrity (SI) functions are interrelated and it is important to know that the PI modifications will improve the SI. Power artifacts impact high speed loads. It is important to understand that the power supply noise results in high speed jitter, which eventually results in bit errors, and one can observe the eye closure.

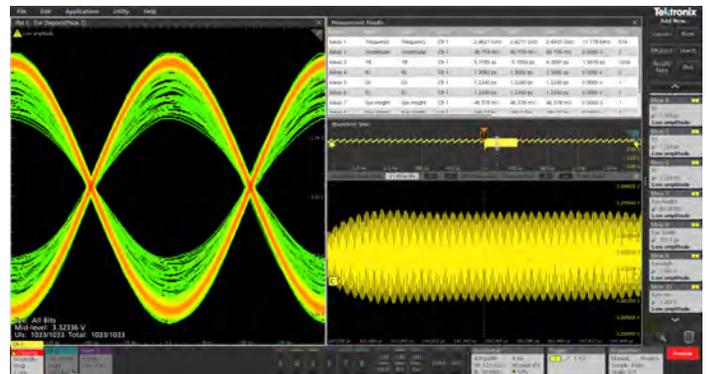

For instance, a SI (Signal Integrity) engineer can measure POL (Point of Load) powering the clock and observe the eye diagram where it is clean and opens up. If the eye diagram is not clean and if there are spurs from POL, then the PI (Power Integrity) engineer can work to modify their power supply design to get better sensitivity. This makes SI engineer see the improvement on the HSS load.



To set up the test, specify the jitter frequency, reference levels, and clock recovery. The Jitter Analysis is included with 5/6-DPM only and is not supported on the 5-DPM-BAS package.

Power Integrity and Signal Integrity analysis


The PSIJ (Power Supply Induced Jitter) is one of the key SI/PI measurement that acts as a tool that gives insights and confidence to the High Speed Serial (HSS) design engineers to improve the designs before making any power related (hardware) changes during the prototyping phase.

This measurement has two goals:

- To identify the jitter caused by the power rail noise
- To suppress the jitter on HSS waveform and see the improvement in the signal quality

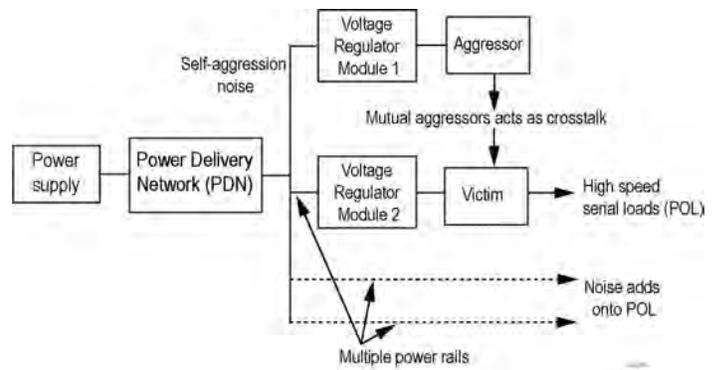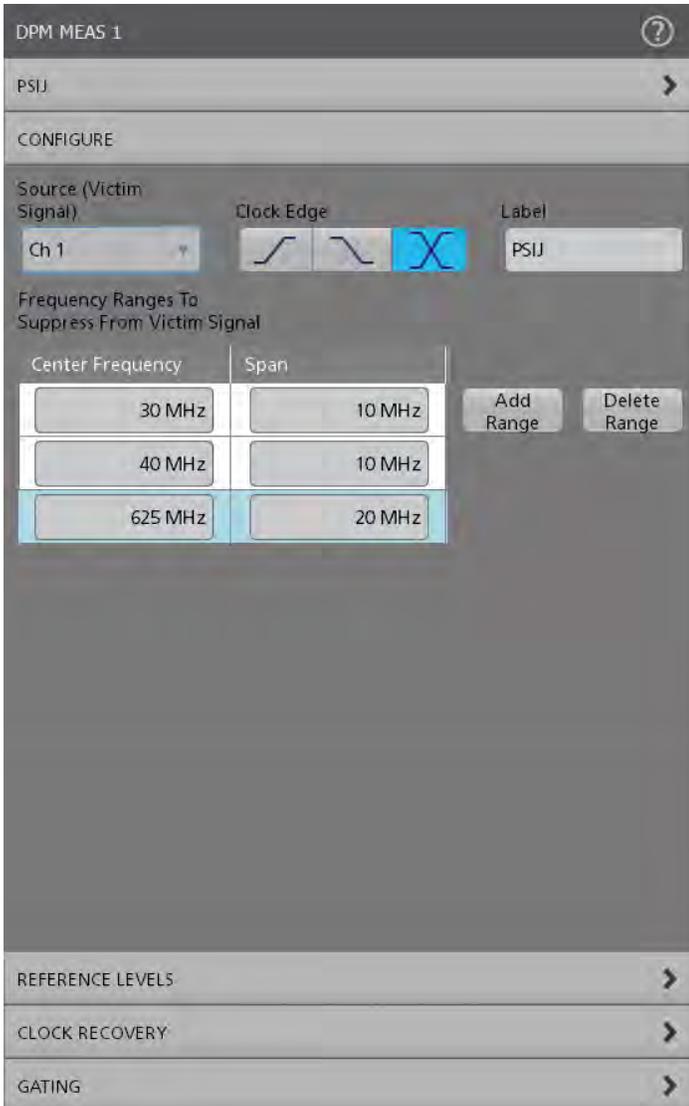

The image shows a multi-rail example of the effect of noise with various points of loads (POL) such as DDR memory, PCIe, etc.

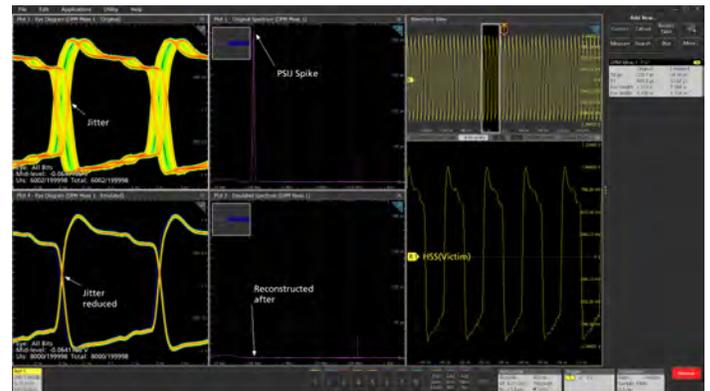

The image shows improvement in PSIJ results after removing the jitter which was added by the power rail source

Report generation

The application allows for data collection, archiving, and documentation necessary for the design and development process. The DPM software provides the ability to compile all the results of a test run into different report formats (MHT or PDF) with pass/fail results for easy analysis.

The PSIJ measurement correlates periodic jitter (PJ) component in high speed signals (victim) with the power supply (aggressor) rail noise using the jitter suppression technique. The jitter suppression algorithm filters out the specified frequencies from the victim signal which were induced from the power rail source. Configure the notch filter with the center frequency that needs to be suppressed from the victim signal. The span of notch filter is an absolute value which specifies spread of notch filter around the center frequency and span. Up to 12 notch filter settings can be configured. It is recommended to run the PSIJ measurement with a constant clock recovery method. The spectrum plots of the HSS before and after filtering out the power rail noise helps to validate the improvement in signal quality. This can also be verified by adding eye diagram plot on the HSS signals.

The measurement gives out essential results such as eye height, eye width, PJ, and TIE of the original and emulated signals.

Measurement Report **Teltronix**

Setup Configuration

| Scope Details | | | |
|--------------------|---------------------|------------------|--------------------------|
| Scope Model Number | Scope Serial Number | TekScope Version | Scope Calibration Status |
| MSO58 | Q100118 | 1.23.22 | Pass |


| Probe Details - CH1 | | |
|---------------------|---------------------|------------------|
| Probe Type | Probe Serial Number | Probe Cal Status |
| TPR4000 | KR01021 | Default |

| Probe Details - CH8 | | |
|---------------------|---------------------|------------------|
| Probe Type | Probe Serial Number | Probe Cal Status |
| TPP0592 | C000119 | Default |

Measurement Result Details

| Name | Measurement | Src(s) | Mean | Min | Max | Pk-Pk | Std Dev | Populatio n | Accum Mean | Accum Min | Accum Max | Accum Pk-Pk | Accum Std Dev | Accum Pop |
|------------------|-------------|---------------|-----------|------------|-----------|-----------|-----------|----------------|---------------|--------------|--------------|----------------|------------------|--------------|
| DPM Meas 1 - TIE | Power | Ch 1 - Rail 1 | 3.7852 us | -26.139 us | 26.219 us | 52.358 us | 15.283 us | 78 | 3.7852 us | -26.139 us | 26.219 us | 52.358 us | 15.283 us | 78 |
| DPM Meas 3 - RJ | Power | Ch 1 - Rail 1 | 9.3154 us | 9.3154 us | 9.3154 us | 0.0000 s | 0.0000 s | 1 | 9.3154 us | 9.3154 us | 9.3154 us | 0.0000 s | 0.0000 s | 1 |
| DPM Meas 4 - DJ | Power | Ch 1 - Rail 1 | 68.530 us | 68.530 us | 68.530 us | 0.0000 s | 0.0000 s | 1 | 68.530 us | 68.530 us | 68.530 us | 0.0000 s | 0.0000 s | 1 |

Views
Time Domain View

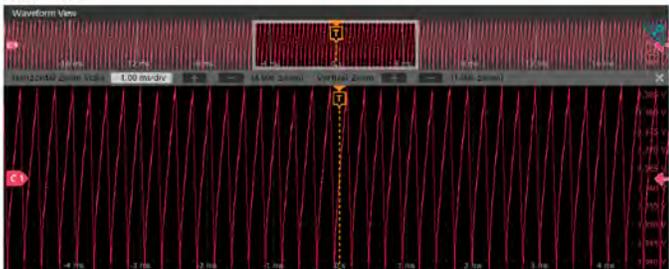

Specifications

| | |
|--|---|
| Ripple analysis | <p>Based on the oscilloscope and the power rail probes used, the ripple varies:</p> <ul style="list-style-type: none"> • <10 mV (MSO6x) • >10 mV (MSO5x) <p>Spectrum View enables to identify the source of ripple Set bandwidth limit from the measurements Configure ripple frequency for each power rail</p> |
| Transient analysis | <p>Measurements include Overshoot, Turn on Undershoot, and DC Rail Voltage Allows designers to enter voltage levels and reference voltage levels for calculating overshoot and undershoot Set bandwidth limit from the measurements</p> |
| Power sequence analysis | <p>Turn on and Turn off times testing enables designers to find out the Turn on or Turn off times of all rails in one go Allows designers to configure the capture time</p> |
| Jitter analysis (available on 5/6-DPM only) | <p>Measurements include TIE, RJ, DJ, PJ, Eye High, Eye Low, Eye Height, and Eye Width Capture jitter across multiple rails at one go</p> |
| PI/SI analysis | <p>PSIJ measurement to identify the periodic jitter introduced on the high speed serial data due to the power rail noise</p> |
| Plots | <p>Eye diagram, Spectrum, and Histogram</p> |
| Report | <p>MHT and PDF format Raw data can be exported to CSV format</p> |
| Degauss / Deskew (static) | <p>Automatic detection of probes Auto Zero: allows to deskew probes from the menu of each channel Manually deskew from the menus for each channel</p> |
| Source support | <p>Live analog signals, reference waveforms, and math waveforms</p> |

Ordering information

Models

| Product | Options | Supported instruments | Bandwidth available |
|--|---|---|--|
| New instrument | 5-DPMBAS (Jitter package not included) | 5 Series B MSO (MSO54B, MSO56B, MSO58B) | <ul style="list-style-type: none"> • 350 MHz • 500 MHz • 1 GHz • 2 GHz |
| | 5-DPM | 5 Series B MSO (MSO54B, MSO56B, MSO58B) | |
| | | 5 Series MSO Low Profile (MSO58LP) | |
| 6-DPM | 6 Series B MSO (MSO64B, MSO66B, MSO68B) | <ul style="list-style-type: none"> • 1 GHz • 2.5 GHz • 4 GHz • 6 GHz • 8 GHz • 10 GHz | |
| Upgrade software on an existing instrument | SUP5-DPMBAS (Jitter package not included) | 5 Series MSO (MSO54, MSO56, MSO58) | <ul style="list-style-type: none"> • 350 MHz • 500 MHz • 1 GHz • 2 GHz |
| | | 5 Series B MSO (MSO54B, MSO56B, MSO58B) | |
| | SUP5-DPM | 5 Series MSO (MSO54, MSO56, MSO58) | |
| | | 5 Series B MSO (MSO54B, MSO56B, MSO58B) | |
| | | 5 Series MSO Low Profile (MSO58LP) | |
| | SUP6-DPM | 6 Series MSO (MSO64) | |
| 6 Series B MSO (MSO64B, MSO66B, MSO68B) | | | |

Software bundles

| Bundle options | Description | Supported instruments |
|-----------------|------------------------------------|-----------------------|
| 5-PRO-POWER-1Y | 1 Year License Pro Power Bundle | 5 Series B MSO |
| 5-PRO-POWER-PER | Perpetual License Pro Power Bundle | |
| 5-ULTIMATE-1Y | 1 Year License Ultimate Bundle | |
| 5-ULTIMATE-PER | Perpetual License Ultimate Bundle | |

Table continued...

| Bundle options | Description | Supported instruments |
|-----------------|------------------------------------|-----------------------|
| 6-PRO-POWER-1Y | 1 Year License Pro Power Bundle | 6 Series B MSO |
| 6-PRO-POWER-PER | Perpetual License Pro Power Bundle | |
| 6-ULTIMATE-1Y | 1 Year License Ultimate Bundle | |
| 6-ULTIMATE-PER | Perpetual License Ultimate Bundle | |

Recommended probes

| Probe type | Nomenclature | Probe bandwidth |
|-------------------|--------------|-----------------|
| Power Rail Probes | TPR1000 | 1 GHz Probe |
| | TPR4000 | 4 GHz Probe |

Note:

- TPR1000 and TPR4000 are the recommended probes for the DPM measurement. The TPR1000 and TPR4000 probes and oscilloscope provides a low-noise measurement solution. The higher input impedance in the probes minimizes the oscilloscope loading effect on the DC rails (50 kΩ at DC).
- Do not confuse the noise of the oscilloscope and probe with the noise and ripple of the measured DC supply.
- P6150 and Direct SMA cable with DC Block can also be used for power rail measurement.



Tektronix is ISO 14001:2015 and ISO 9001:2015 certified by DEKRA.



Product(s) complies with IEEE Standard 488.1-1987, RS-232-C, and with Tektronix Standard Codes and Formats.

ASEAN / Australasia (65) 6356 3900
 Belgium 00800 2255 4835*
 Central East Europe and the Baltics +41 52 675 3777
 Finland +41 52 675 3777
 Hong Kong 400 820 5835
 Japan 81 (120) 441 046
 Middle East, Asia, and North Africa +41 52 675 3777
 People's Republic of China 400 820 5835
 Republic of Korea +82 2 565 1455
 Spain 00800 2255 4835*
 Taiwan 886 (2) 2656 6688

Austria 00800 2255 4835*
 Brazil +55 (11) 3759 7627
 Central Europe & Greece +41 52 675 3777
 France 00800 2255 4835*
 India 000 800 650 1835
 Luxembourg +41 52 675 3777
 The Netherlands 00800 2255 4835*
 Poland +41 52 675 3777
 Russia & CIS +7 (495) 6647564
 Sweden 00800 2255 4835*
 United Kingdom & Ireland 00800 2255 4835*

Balkans, Israel, South Africa and other ISE Countries +41 52 675 3777
 Canada 1 800 833 9200
 Denmark +45 80 88 1401
 Germany 00800 2255 4835*
 Italy 00800 2255 4835*
 Mexico, Central/South America & Caribbean 52 (55) 56 04 50 90
 Norway 800 16098
 Portugal 80 08 12370
 South Africa +41 52 675 3777
 Switzerland 00800 2255 4835*
 USA 1 800 833 9200

* European toll-free number. If not accessible, call: +41 52 675 3777

For Further Information. Tektronix maintains a comprehensive, constantly expanding collection of application notes, technical briefs and other resources to help engineers working on the cutting edge of technology. Please visit www.tek.com.

Copyright © Tektronix, Inc. All rights reserved. Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specification and price change privileges reserved. TEKTRONIX and TEK are registered trademarks of Tektronix, Inc. All other trade names referenced are the service marks, trademarks, or registered trademarks of their respective companies.