


Advanced Power Measurement and Analysis

4/5/6 Series B MSO Option 4-PWR, 5-PWR, and 6-PWR Application Datasheet

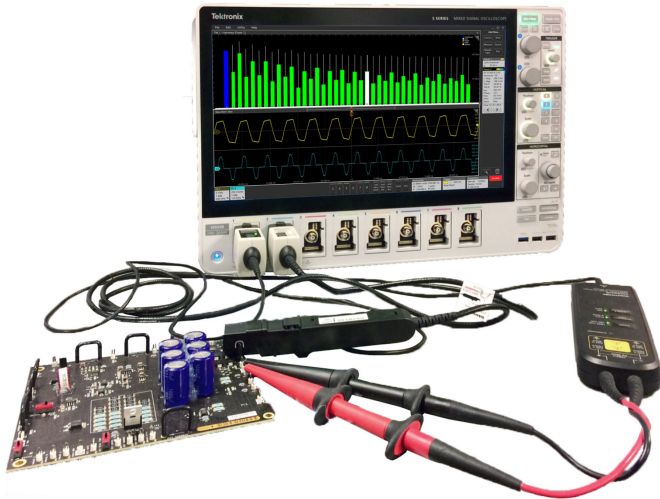

Get more visibility into your power systems with Advanced Power Measurement and Analysis on the 4/5/6 Series B MSO. The combination of the oscilloscope, analysis software, and a wide range of available voltage and current probes, enables you to perform automated, accurate power system measurements even if you are not a power conversion guru. The 12-bit analog-to-digital converters in these oscilloscopes deliver high-precision measurement data, and the pinch/swipe/zoom touch interface makes it easy to manage measurements. A rich set of graphical power analysis tools, high channel-counts, and large HD displays deliver a comprehensive view of your power system. The instruments support a wide range of voltage and current probes, including state-of-the-art IsoVu™ optically isolated voltage probes. The unmatched common mode rejection of IsoVu probes and the automation of Advanced Power Measurement and Analysis make an unbeatable combination for optimizing the latest GaN and SiC designs.

Key measurements

- **Input measurements**
 - **Power** measures true power, apparent power, power factor, and phase angle
 - **Total Harmonic Distortion and Crest Factor measurements**
 - **Harmonics** measurements, bar charts, and tables
- **Amplitude** provides easy per-cycle measurements of voltage or current, including minimum, maximum, amplitude, and peak-to-peak
- **Input Capacitance** measures the capacitance value using voltage and current signals
- **Inrush Current** measures the peak current
- **Switching Device measurements**
 - **Switching Loss** measures turn-on, turn-off, and conduction loss in switching devices
 - **Safe Operating Area (SOA)** provides customizable safe operating area mask testing
 - **Timing Analysis** enables easy analysis of pulse-width-modulated switching signals with cycle-by-cycle plots or histograms of pulse width, duty cycle, frequency, or period
 - **RDS(on)** measures the dynamic resistance of the switching device when it is in the On state
- **Magnetic Analysis measurements (available only in 4/5/6-PWR)**
 - **Inductance** measures inductance of the core
 - **Magnetic Property** measures and plots the inductor B - H curve.
 - **Magnetic Loss** measures and calculates total magnetic loss
 - **I vs. jV** displays the plot of I and jV waveforms
- **Output measurements**
 - **Line Ripple** measures the amount of AC signal related to the input line frequency.
 - **Switching Ripple** measures the amount of AC signal related to the switching frequency.
 - **Efficiency** measures the power circuit efficiency by dividing the measured output power by the measured input power
 - **Turn On Time** measures the time delay between the input voltage to the device under test going 'high' to the output voltage reaching its steady state.
 - **Turn Off Time** measures the time delay between the input voltage to the device under test going to zero state, to the output voltage reaching its zero state.
- **Frequency response measurements(available only in 4/5/6-PWR)**

- **Control Loop Response (Bode)** plots the frequency and phase response of a closed loop circuit, and automatically calculates the gain and the phase margins.
- **Power Supply Rejection Ratio (PSRR)** analyzes the ripple rejection capability of a DC-DC converter.
- **Impedance Analysis** enables 2-port impedance measurement of Power Distribution Networks(PDN) using the oscilloscope.
- **Green Power measurements**
 - **LVRT(Low voltage ride through)** measures how quickly a solar inverter recovers from an intermittent low voltage conditions on the grid.
 - **HVRT(High voltage ride through)** evaluates the inverter recovery behavior during intermittent high voltage events in the connected grid.

Key features

- Add, configure, and remove automated measurements using the 4/5/6 Series B MSO's pinch/swipe/zoom touch interface
- Easily document test results with automated report generation, including measurements, test results, and plots in a single, editable mht file or pdf file
- Utilizes optional and integrated Arbitrary/Function Generator for frequency response analysis (available only in 4/5/6-PWR). Also supports external AFG31000 Series function generator.
- Cover diverse applications with a wide range of voltage and current probes, including state-of-the-art IsoVu optically isolated voltage probes
- Configure any measurement and transfer any result via remote interface for automated testing applications
- Supports Save/Recall function of the session files for the FRA measurements
- Integrated Spectrum View analysis with Power FRA measurements
- When Spectrum View is selected as the analysis method, all FRA measurements supports minimum start frequency of 0.1 Hz, enabling precise low-frequency characterization for sensitive tests.
- FRA measurements supports AWG5200 and AWG70000 Series as external generators, the maximum stop frequency is extended to 1GHz allowing broader bandwidth testing and precise high-frequency characterization.

Input analysis


Power quality measurements, Current Harmonics, Input Capacitance, and Inrush Current are the four common sets of measurements made on the input section of a power supply, to analyze the effects of the power supply on the power line and evaluate the performance of the supply under various line conditions.

Power Quality

These measurements are optimized for line frequencies and are commonly performed at the AC line input of the power supply. They provide fast insight into the amount of power and the level of distortion at the input.

Measurements include:

- RMS voltage and current
- Frequency
- True, apparent, and reactive power
- Power factor
- Crest factors of Voltage and Current

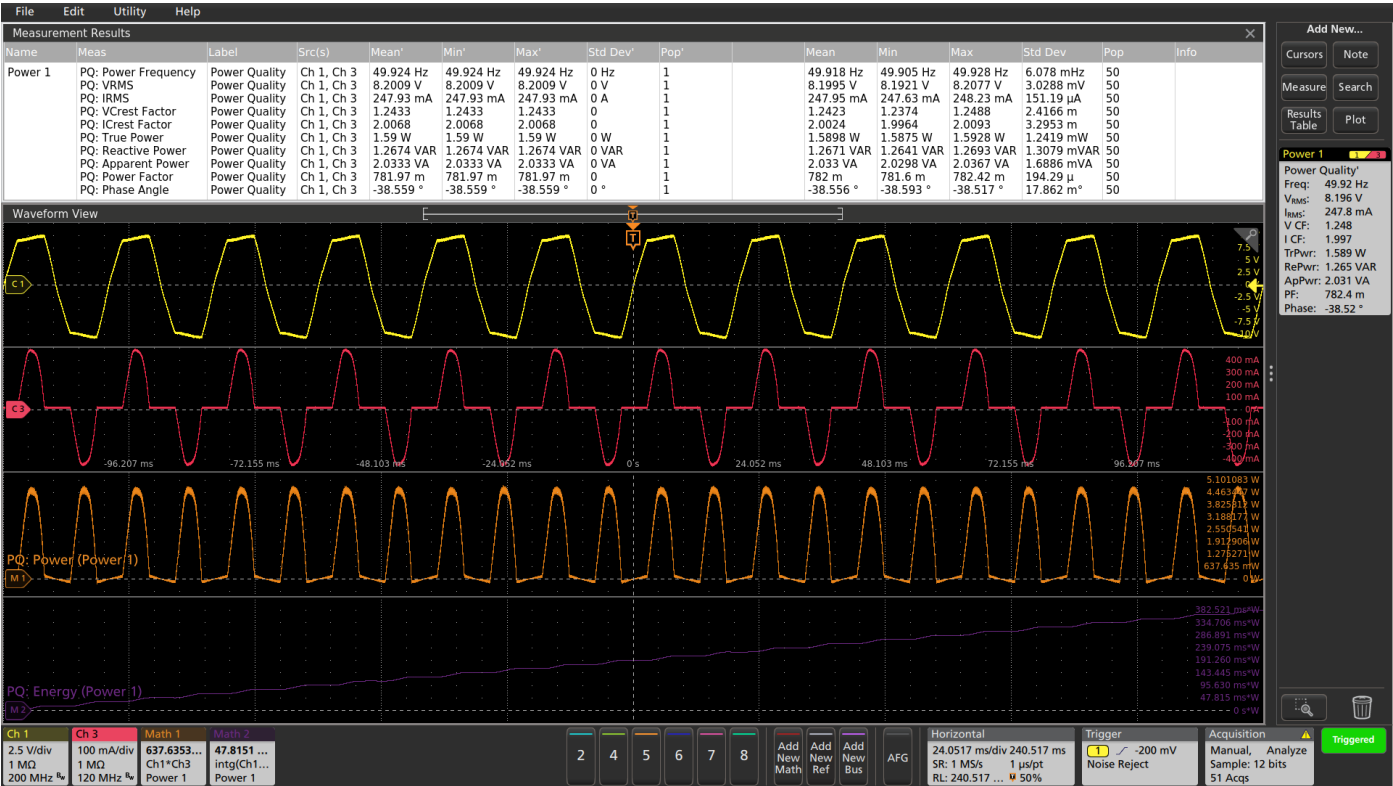


Power Quality measurements deliver information in multiple formats. Numerical results (upper right), tables (upper), and instantaneous power waveform and energy plots (lower).

Harmonics

Any power supply with a non-linear device on its input (e.g. a rectifier) presents a nonlinear load to the AC line. Unless mitigated, excessive harmonic energy can affect the operation of other equipment connected to the power line and increase the cost of delivering the electric power. This has resulted in standards limiting harmonics generated by line-powered devices.

Limits will assist with upcoming new standards and designs when limits are still being defined. With the Custom option, you can set and modify the limits. Power Harmonics computes up to the 400th order harmonics and displays them as bar graphs and also in tabular formats. This lets you easily navigate between the table results and individual harmonics on the bar graph, act as a powerful debug step.

Advanced Power Measurement and Analysis include the test limits for IEC61000-3-2, AM 14, MIL- STD-1399, DO-160, and Custom standards. These standards help you perform pre-compliance testing before investing in official compliance testing. The Custom

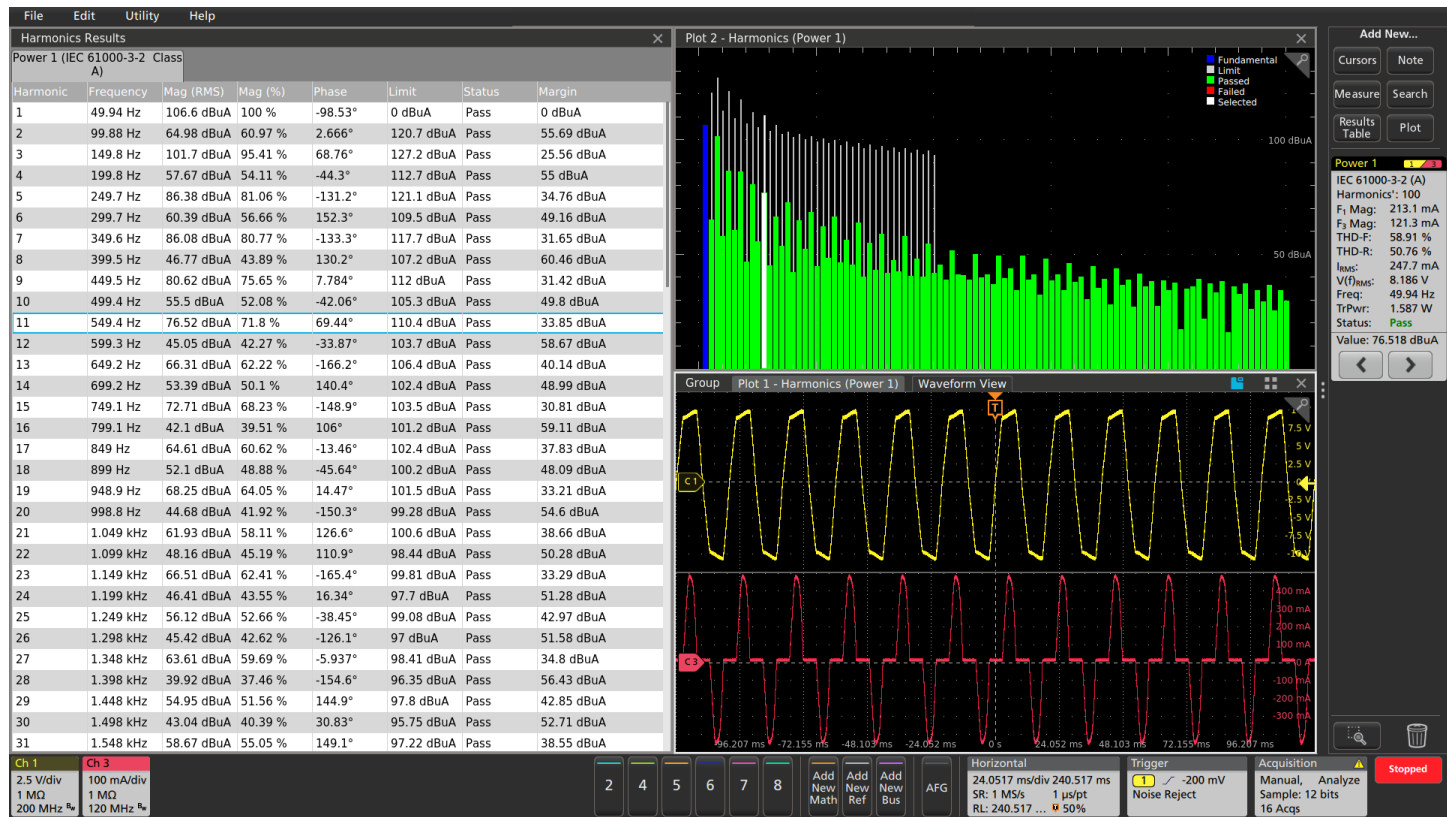


Harmonics bar graph, harmonics results table, and traverse capability via the results bar (upper right).

Input capacitance and Inrush current measurement

4-PWR-BAS, 4-PWR, 5-PWR, and 6-PWR provides peak inrush current and capacitance measurements for testing switching power supplies during operation.

Inrush current, input surge current or switch-on surge is the maximum, instantaneous input current drawn by an electrical device when first turned on. Power converters have inrush current that is more than their steady state current due to the charging current of input capacitance. Measuring inrush current and input capacitance is important to ensure the design works effectively.

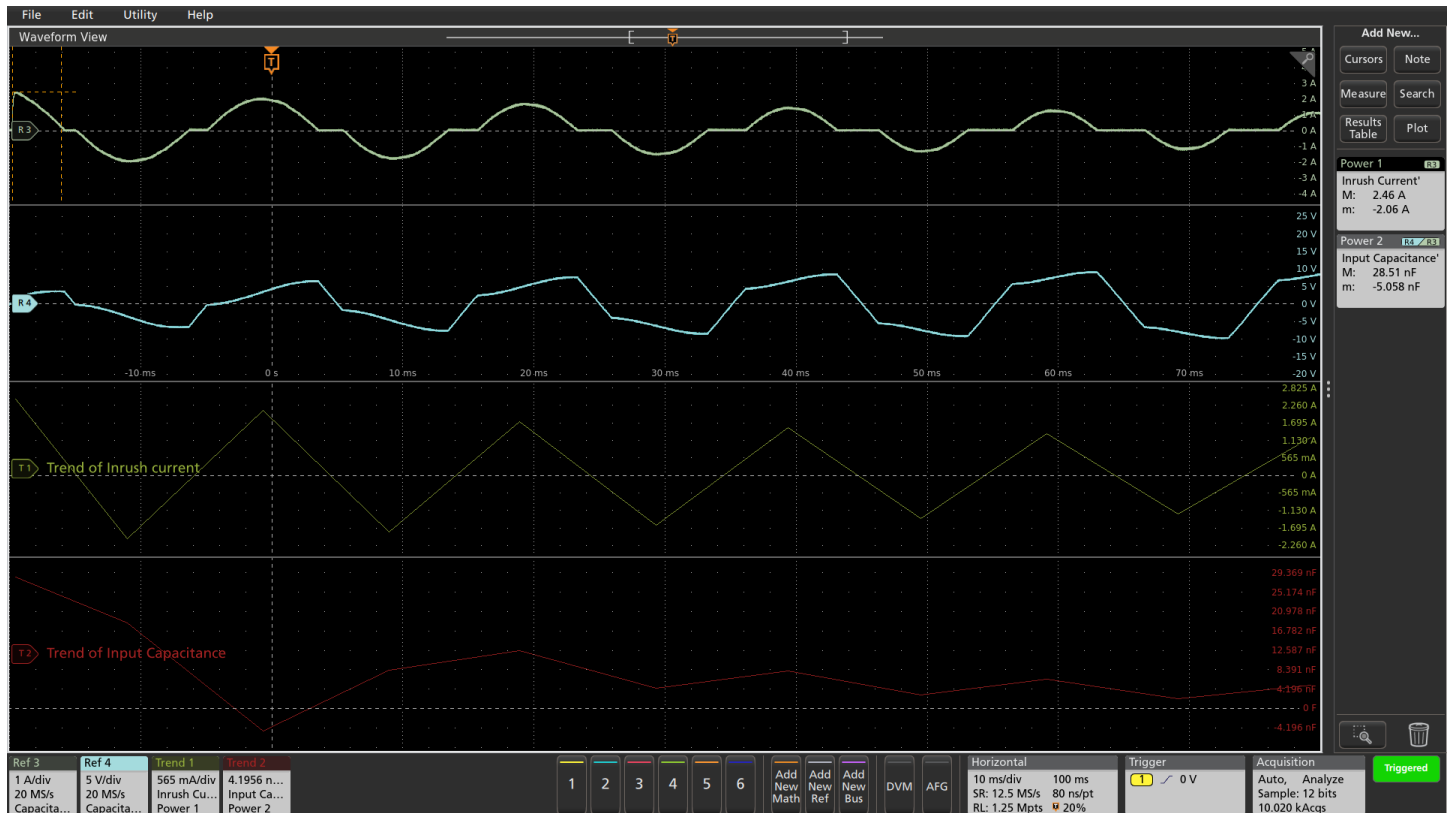

Input capacitance and inrush current measurement with traverse capability.

Switching component analysis

The accurate calculation and evaluation of energy loss in power supplies has become even more critical with the drive toward higher power conversion efficiency and greater reliability.


Switching loss measurements

Although almost all components of a power supply contribute to energy losses, a significant portion of energy losses in a switch-mode power supply (SMPS) occur when the switching transistor transitions from a Turn-off (T_{off}) to a Turn-on (T_{on}) state and vice versa (Turn-off loss). By measuring the voltage drop across the switching device and the current flowing through the switching device, Advance Power Analysis automatically calculates switching loss measurement parameters for each cycle.

Until recently, taking switching measurements on the high side of half-bridge switching stages were almost impossible. Any measurement relative to the switching node, including high-side V_{DS} and voltages across current shunts, suffered from distortion

due to the significant common-mode voltage signal impinging on the differential signal. This problem is worse with wide bandgap devices, such as GaN and SiC transistors, as switching frequencies increase and the need to optimize new designs becomes imperative.


The 4/5/6 Series B MSO is designed to work with IsoVu optically isolated probes, enabling designers to perform accurate switching measurements even in the presence of high common mode signals.

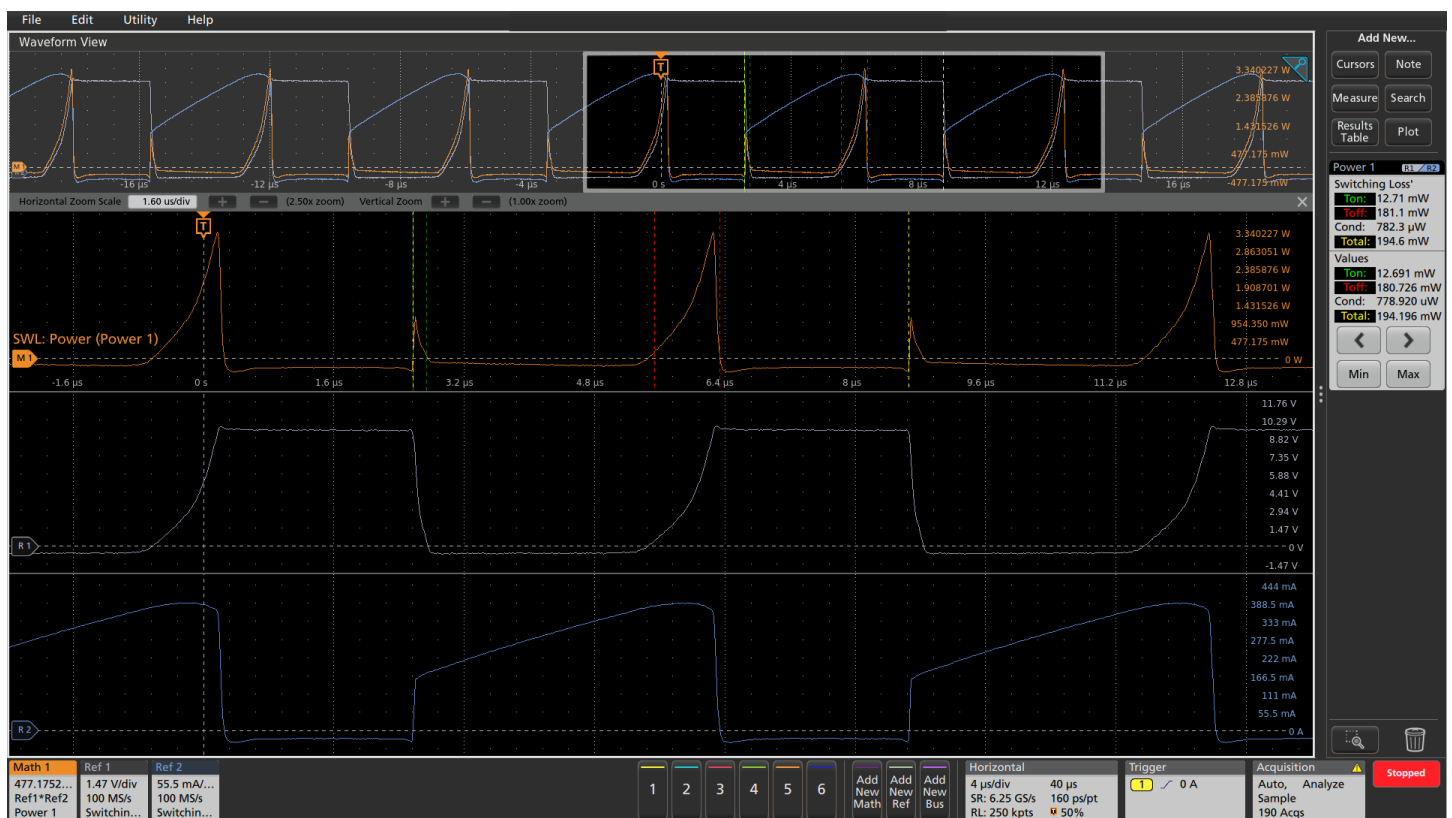

Switching Loss shows FET power dissipation. Waveforms are marked with color-coded markers showing the measurement regions for Ton, Toff, and Total cycle, that match the results badge. Controls in the results badge let you traverse from cycle to cycle.

Switching loss measurements include special settings to produce stable, repeatable measurements on active power factor correction stages, and flyback converters.

To get an overview of the switching loss for all captured cycles, you can use the trajectory plot. It automatically plots the voltage across the switch versus current through the switch during turn-on and turn-off, letting you judge the range of switching loss for all cycles at a glance.

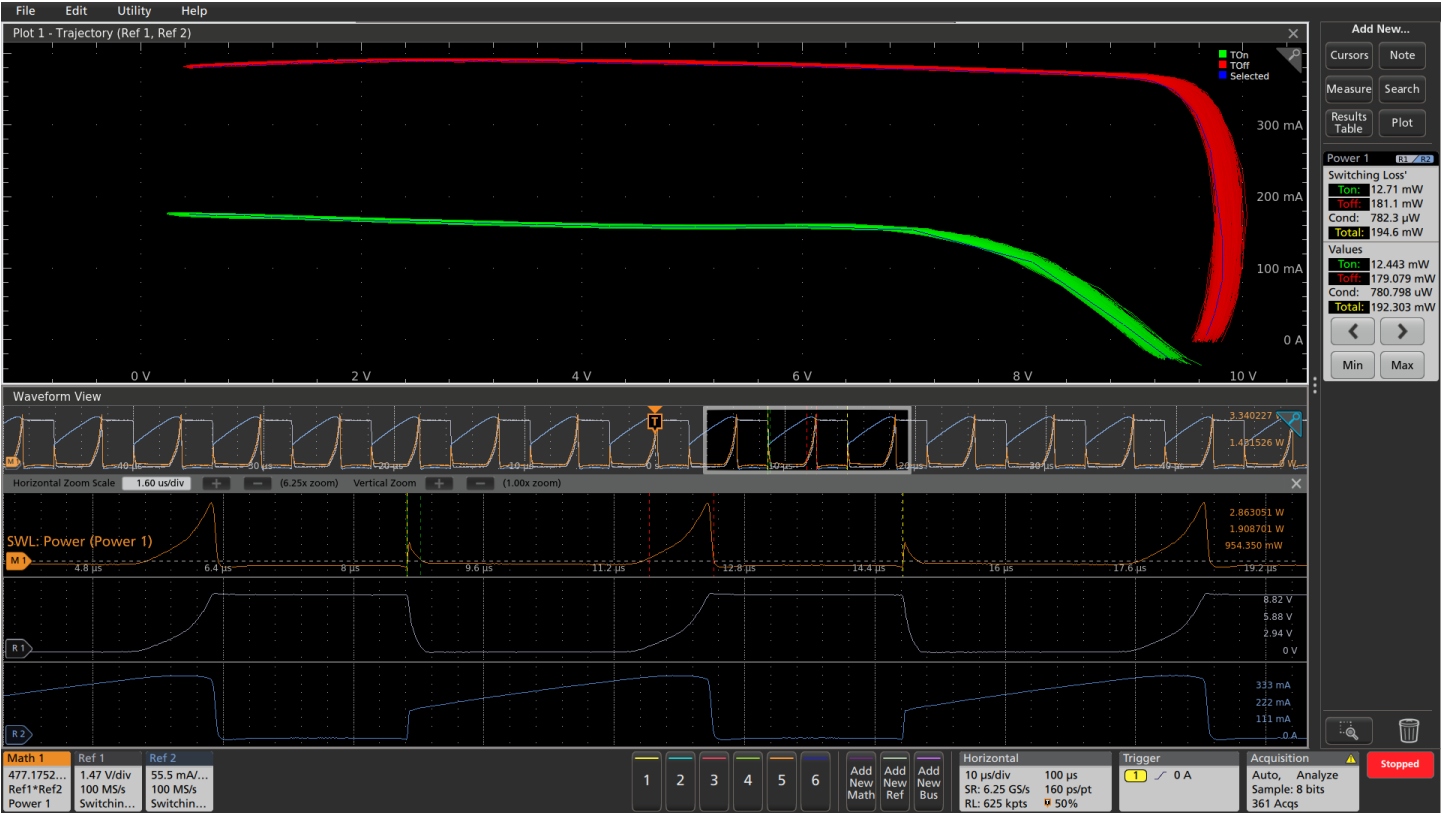


Switching Loss Trajectory Plots (upper window) show the Ton loss, and Toff loss for all switching cycles in a single plot.

Safe operating area

The Safe Operating Area (SOA) plot is a graphical technique for evaluating a switching device to ensure that it is not being stressed beyond its maximum specifications. SOA testing can be used to validate performance over a range of operating conditions,

including load variations, temperature changes, and variations in input voltages. Mask testing can also be used with SOA plots to automate validation.

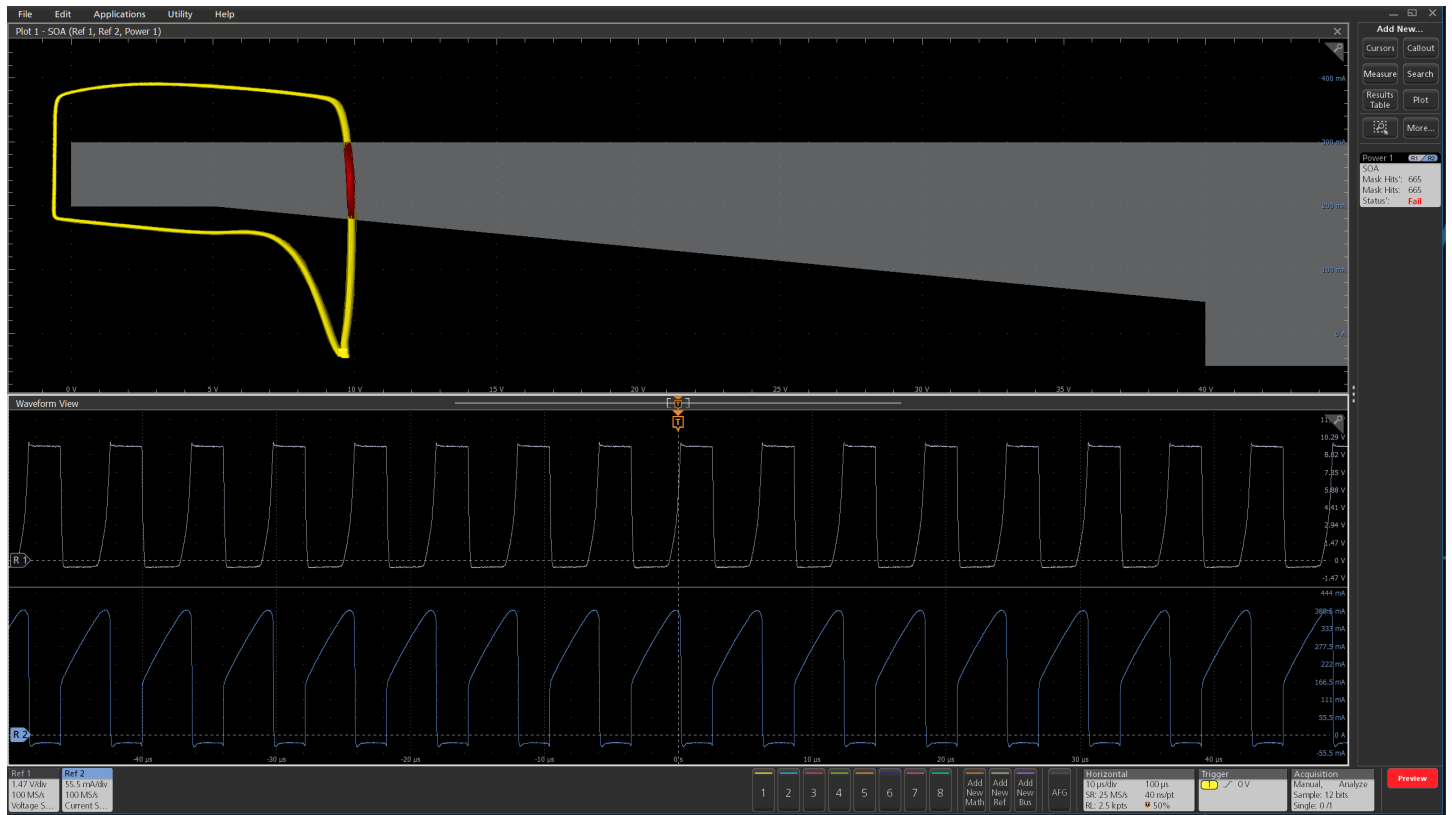


Safe Operating Area (SOA) plot with mask helps verify the switching devices are staying within their SOA envelope under changing operating conditions.

RDS(on)

This measurement characterizes the resistance of the switching device during the conduction cycle, when the device is ON and conducting current. The dynamic-on-resistance is the ratio of the voltage across the device when it is turned ON to the current

flowing through the device. The software ensures that the minimum RDS_{on} value in the acquisition is highlighted and zoomed in for easy viewing. In addition, the traverse capability helps to move from cycle to cycle to the respective RDS_{on} values.

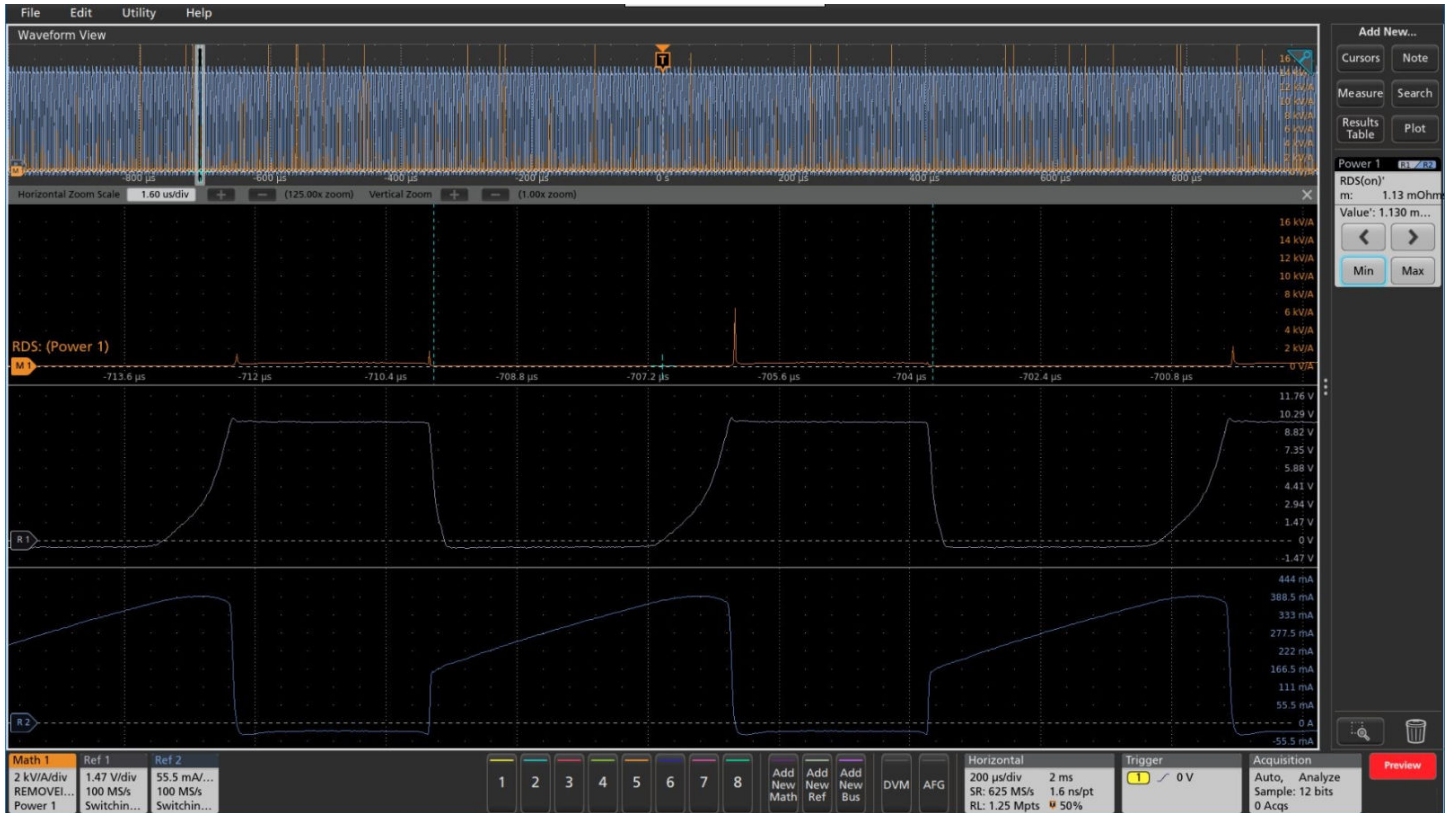

RDS(on) measurement

Magnetic analysis (available only in 4/5/6-PWR)

Supports the following measurements:

- Inductance
- Magnetic property including BH curve
- Magnetic loss
- I vs. $\int V$

Magnetic components are an important part of any power supply system. Inductors and transformers are used as energy storage devices in both switch-mode and linear power supplies. Some power supplies also use Inductors in filters at their output stage. Given their important role in the system, it is essential to characterize these magnetic components to determine the stability and overall efficiency of the power supply.

Inductance

Inductors exhibit increasing impedance as frequency increases, impeding higher frequencies more than lower frequencies. This behavior is known as inductance and is measured in units of Henries. The inductance can be measured automatically with Advanced Power Measurement and Analysis software.

Magnetic loss

An analysis of magnetic power losses is essential to accurately characterize the efficiency, reliability, and performance of a switching power supply. Advanced Power Measurement and Analysis software measures the inductive total magnetic power loss, as shown in the following figure.

Magnetic Property

This measurement computes the properties of the magnetic components including magnetic flux density (B), magnetic field intensity strength (H) and various loss components including Hysteresis Loss and Total Loss. This measurement also supports multiple secondary source configuration based on the scope channel count.


B-H plots

The properties of magnetic materials are described by the magnetic flux density (B), magnetic field intensity strength (H), and the magnetic permeability of a material (μ). B-H plots are often used to verify the saturation (or lack thereof) of the magnetic elements in a switching supply and provide a measure of the

energy lost per cycle in a unit volume of core material. Advanced Power Measurement and Analysis software measures the voltage across the magnetic element and the current flowing through it, and plots B versus H, as shown in the following figure. You can test multiple secondary windings of a transformer simultaneously, thereby ensuring faster validation/testing times leading to faster time to market.

I vs. $\int V$ plot

I vs. $\int V$ plot provides insight to the B and H values, proportional to the voltage and current. This is the integral of the voltage and current waveforms in X-Y plot format as shown in the following figure.

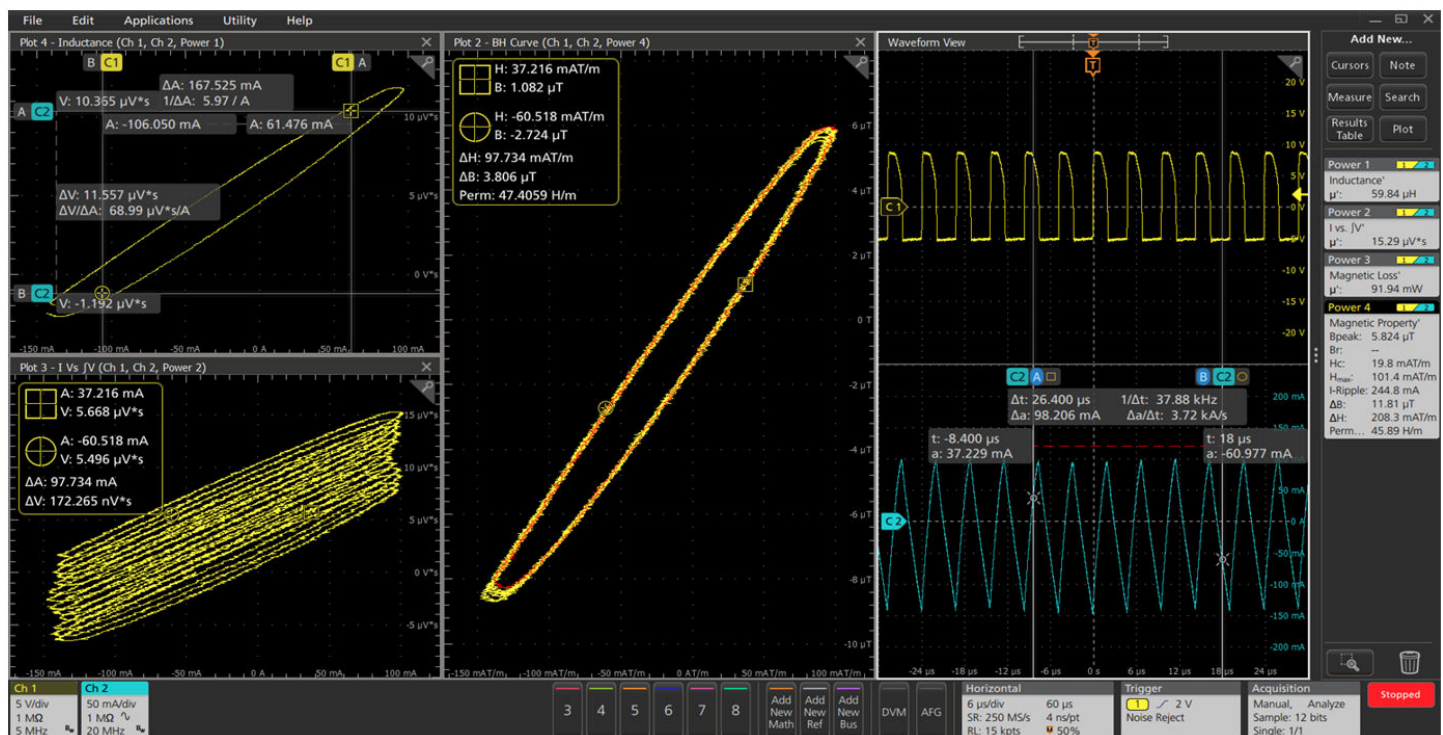

Magnetic Analysis measurement with B-H curve, I vs. $\int V$, and Inductance plots.

Output analysis


The ultimate goal of a DC-output power supply is to transform input power into one or more DC output voltages. The most important output measurements for switching power supplies are line ripple and switching ripple.

Line and switching ripple

The quality of a power supply's DC output should be clean, with minimal AC noise and ripple. Advanced Power Measurements and Analysis software measures ripple to help you isolate the cause.

Line ripple measurements indicate the amount of AC signal

related to the input line frequency (since the input is rectified, line ripple is usually twice the frequency of the AC line). Switching ripple measures the amount of AC signal related to the switching frequency.

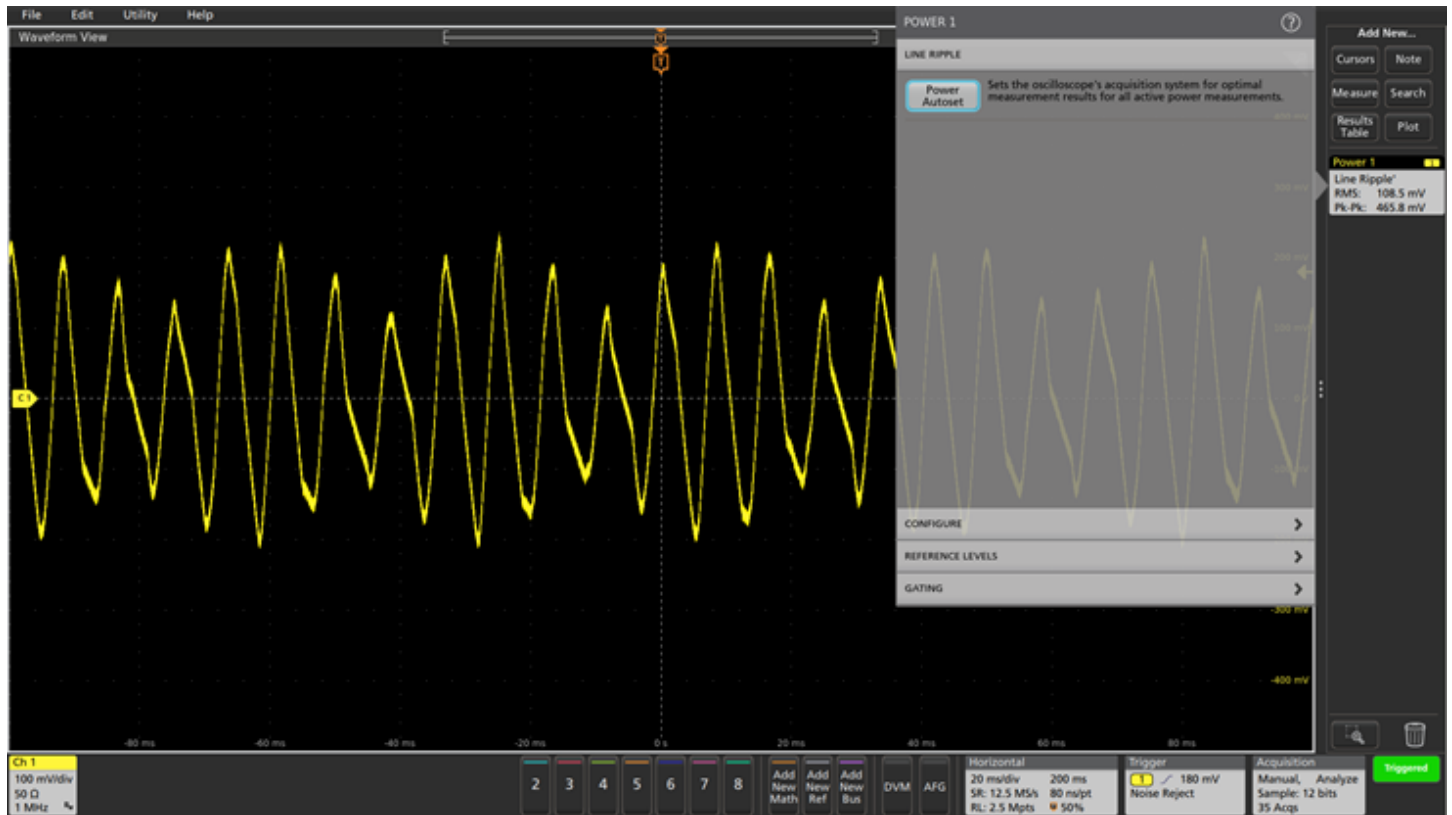


Ripple analysis helps distinguish low-frequency line ripple from higher frequency switching noise.

Efficiency

Device or product efficiency is a critical differentiator in today's competitive environment. Advanced Power Measurements and Analysis software lets you easily measure your product's power conversion efficiency (AC-DC, AC-AC, DC-DC, DC-AC).

It allows you to test efficiency on multiple outputs at once, for faster testing and validation. You can configure each output independently.

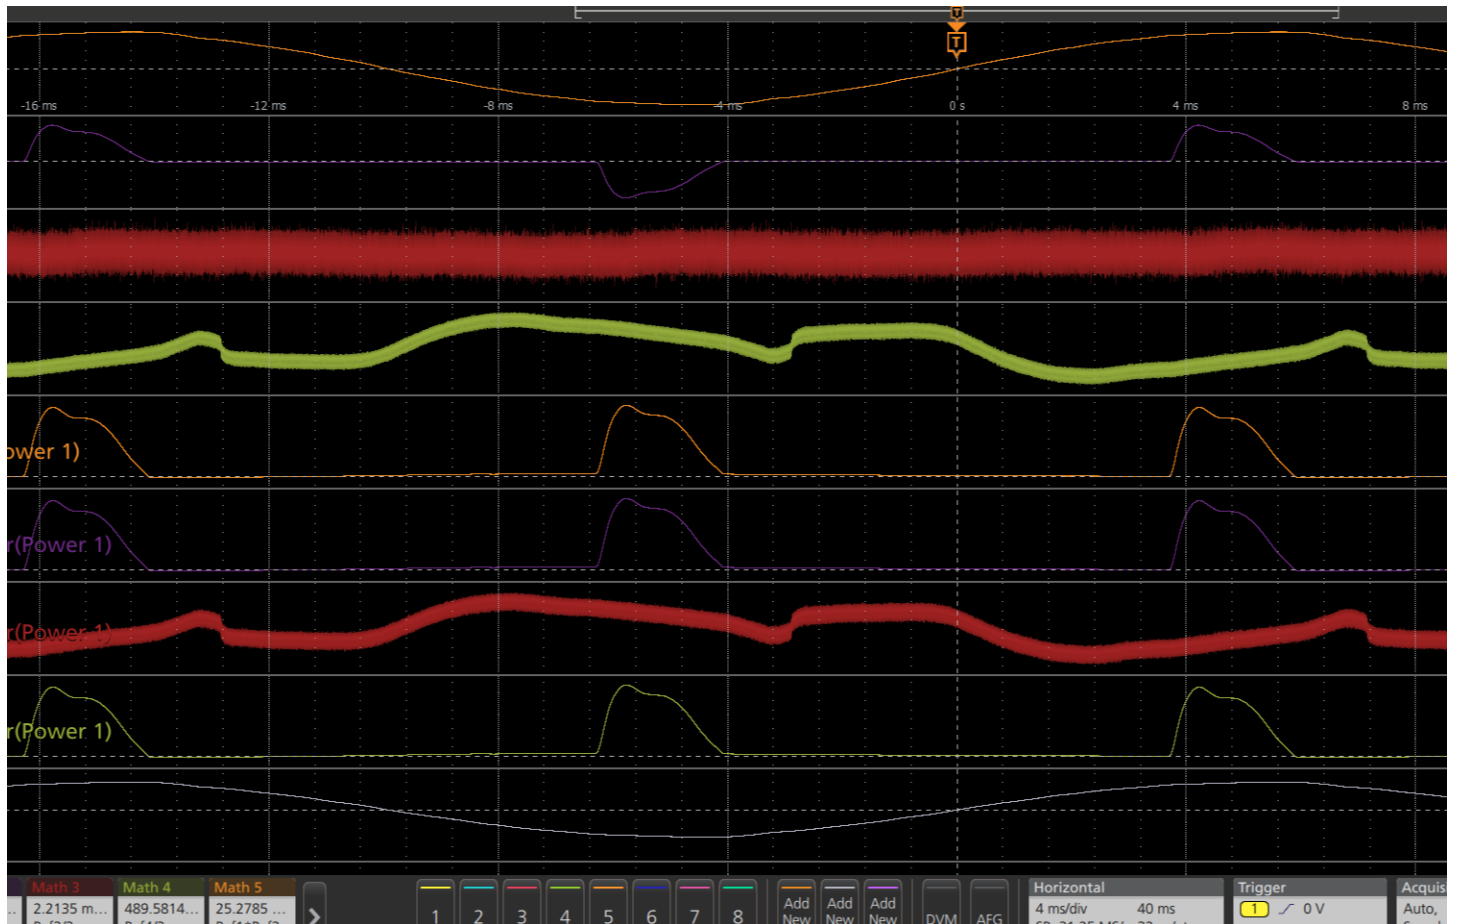

Efficiency measurement

POWER 2

?

EFFICIENCY

CONFIGURE

Input Voltage Source

Ch 1

Input Current Source

Ch 2

Label

Efficiency

Input

AC

DC

Number Of Outputs

1

2

3

Output 1 Voltage

Ch 3

Output 1 Current

Ch 4

Output 1

AC

DC

Output 2 Voltage

Ch 5

Output 2 Current

Ch 6

Output 2

AC

DC

Output 3 Voltage

Ch 7

Output 3 Current

Ch 8

Output 3

AC

DC

REFERENCE LEVELS

GATING

Efficiency measurement configuration lets you test new generation multi-output power conversion devices (AC-DC, AC-AC, DC-DC, and DC-AC).


Turn on time and turn off time

Turn on time is defined as the time it takes for the output voltage to reach a steady state after the input voltage is turned on.


Turn off time is defined as the time it takes for the output to reach its zero state after the input voltage is switched off.

It is very important for SMPS to operate at specified turn on and turn off time. If the delay between mains power and SMPS startup is not as per design (typically 1 ms) it can disrupt the operation of some sensitive loads. Most embedded systems use more than one power supply and many use multiple outputs.


4-PWR-BAS, 4-PWR, 5-PWR, and 6-PWR automates this measurement for up to 5 outputs (4 Series MSO) or up to seven outputs (5 Series MSO or 6 Series B MSOs) or up to 3 outputs (6 Series MSO) simultaneously.

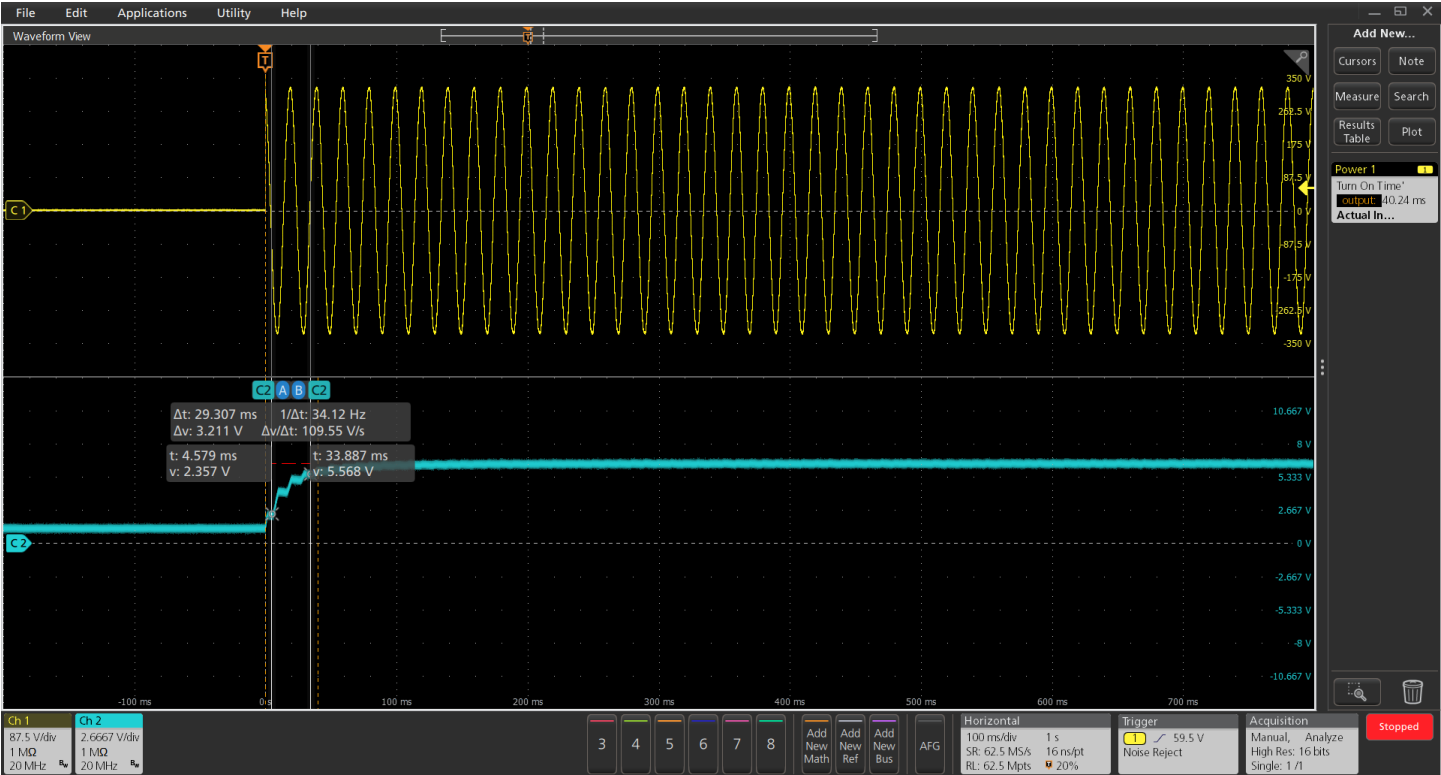

Turn on time measurement

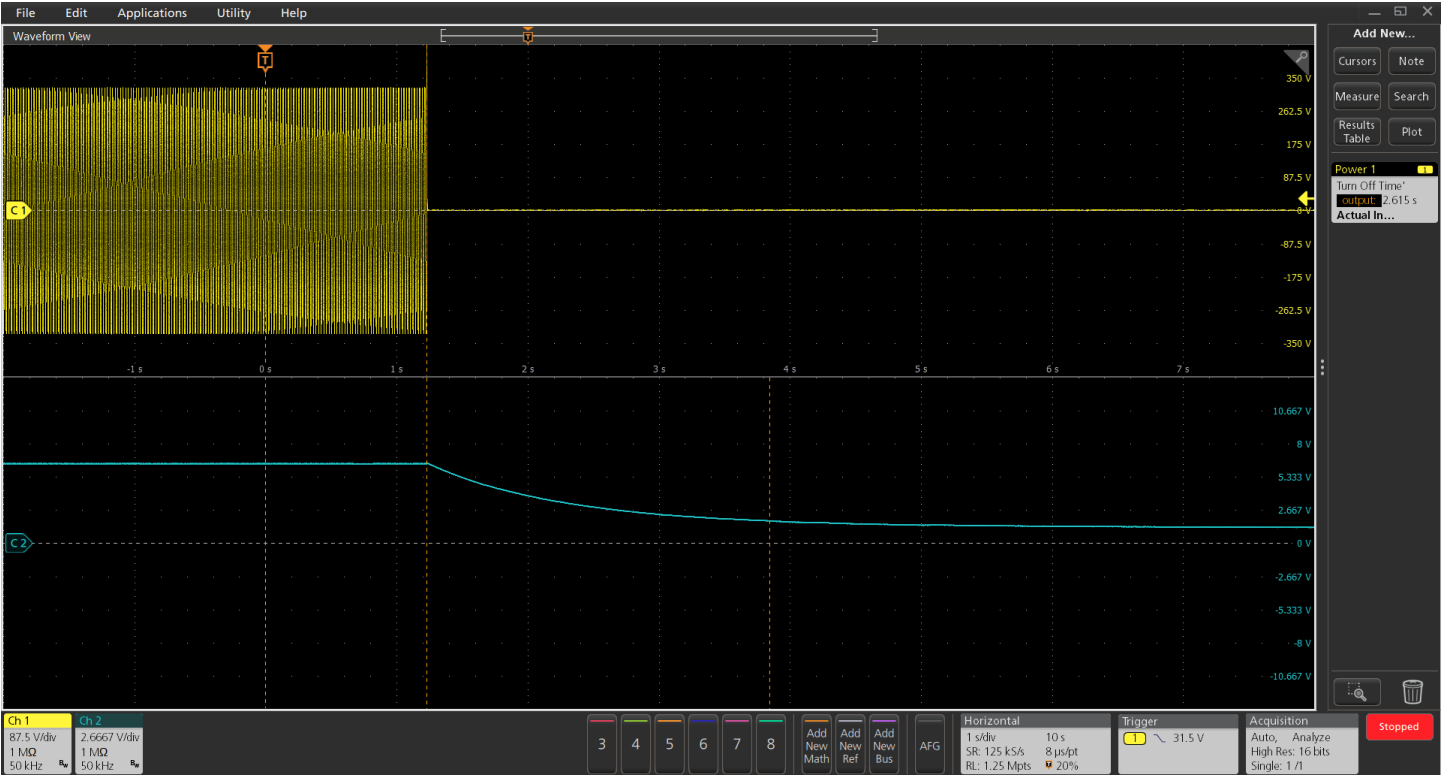

Turn off time measurement

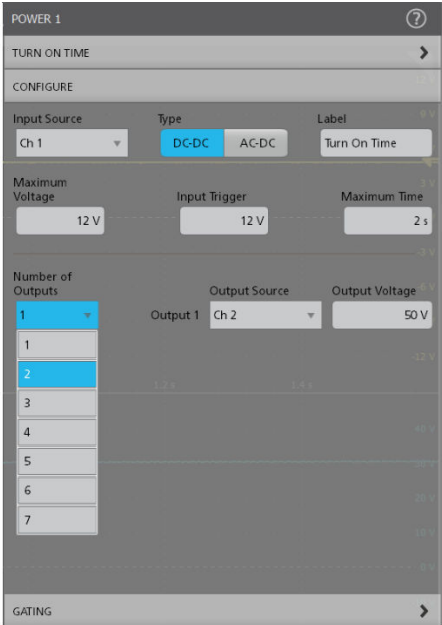

The Turn on time measurement configuration supports multiple output devices.



The Turn off time measurement configuration supports multiple outputs.

Frequency response analysis (available only in 4/5/6-PWR)

The Control Loop Response analysis (Bode plots), Power Supply Rejection Ratio (PSRR) and Impedance measurement provide key measurements to ensure stable, low-noise power supply designs. While it is possible to perform this analysis with a vector network analyzer or dedicated frequency response analyzer, these instruments can require significant setup time and long learning curves. Advanced Power Measurement and Analysis enables frequency response analysis on 4/5/6 Series MSOs using either the optional built-in AFG (4/5/6-AFG option) or an external AFG31000 Series function generator.

These measurements leverage the built-in Spectrum View tool on the 4/5/6 Series B MSOs to get a finer frequency resolution across the various user-configurable frequency bands, and improve the accuracy of test results by analyzing the measurements in the frequency domain.

Control Loop Response (Bode plots)

Bode plots and gain/phase margin measurements enable designers to determine the stability of a power supply control loop. Unstable control loops lead to oscillations and inefficient performance. Filter designers also use amplitude and phase plots to test filter designs.

Automated Control Loop Response measurements use the built-in AFG to provide a single source to sweep through a specified frequency range, plotting amplitude and phase at each point. Signals are introduced into the control loop using an injection transformer, such as the J21xxA models from Picotest. The resulting gain and phase plots (Bode plots) are used to automatically calculate gain and phase margins. Cursors allow you to view gain and phase values at any frequency on the curves.

Control Loop Response measurement allows you to set START and STOP frequencies using the optional built-in AFG (requires 4/5/6-AFG option) or an external AFG31000 Series function generator, select constant/amplitude profile, impedance, phase wrap, analysis method as FFT, Spectrum Average, and Spectrum Normal, and points per decade for better plot rendering.

Phase Wrap configuration allows you to unwrap the phase trace where it jumps more than the number of degrees set in the adjacent field. The default phase is set to 180°.

POWER 1 ⓘ

CONTROL LOOP RESPONSE

Input Source: Ch 1 ▾ Output Source: Ch 2 ▾ Label: Control Loop Re...

Generator: Internal (selected) External Impedance: 50 Ω (selected) High Z


Analysis Method: Spectrum Average ▾ Start Frequency: 100 Hz Stop Frequency: 20 MHz

Sweep Profile: Auto (selected) Custom Constant Amplitude: 100 mV Points Per Decade: 10

Phase Wrap: ☐

Go Upon pressing Go, the oscilloscope will configure itself and the signal generator to create the desired plot based on the inputs above.

Control Loop Response measurement allows you to set START and STOP frequencies using the optional built-in AFG (requires 4/5/6-AFG option) or an external AFG31000 Series function generator.

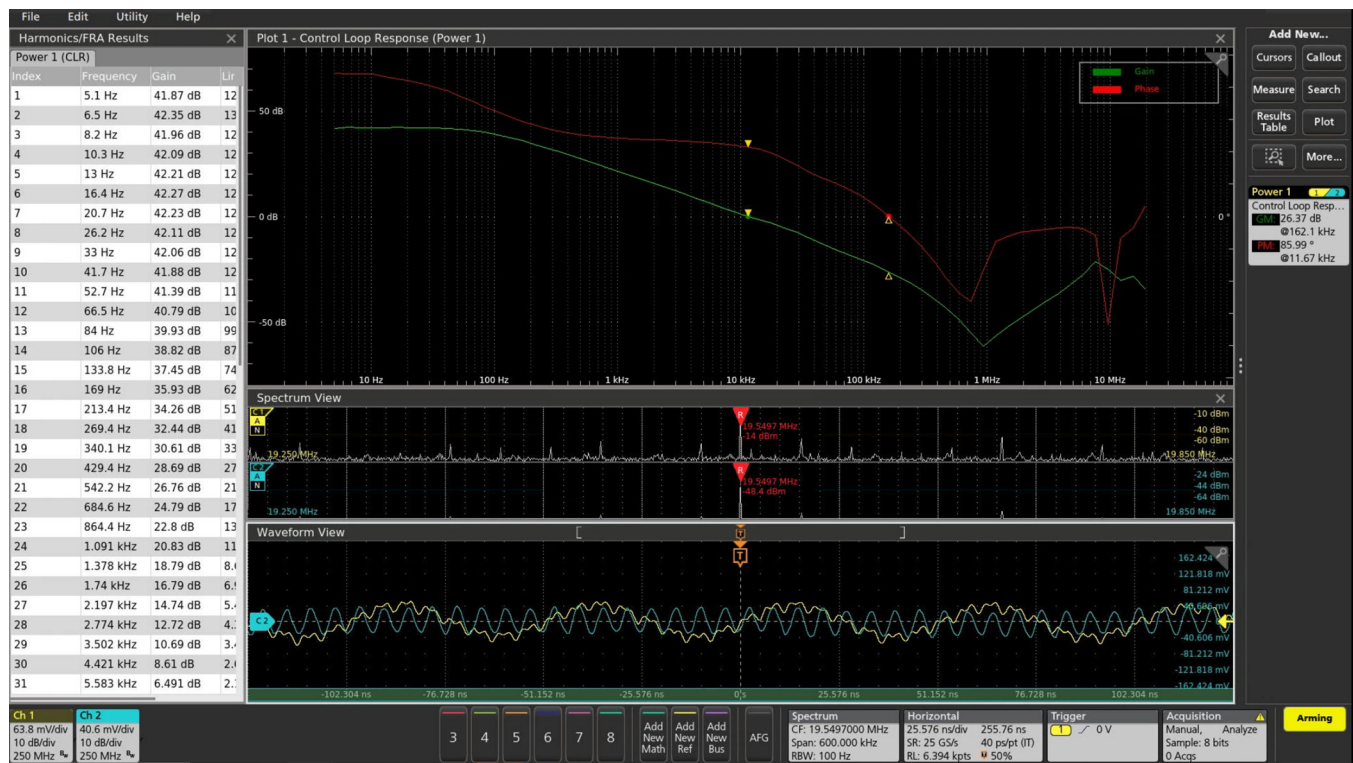

Control Loop Response (Bode plot) plots gain and phase versus frequency and calculates the gain margin and phase margin.

Power Supply Rejection Ratio (PSRR)

The PSRR measurements enable designers of DC-DC converters and regulators to quantify the ability of devices to attenuate AC over a specified frequency range. The test uses the optional, built-in function generator of the 4/5/6 Series B MSO or an external Tektronix AFG31000 function generator, along with an injection transformer (such as the Picotest J2120A Line Injector), to modulate the input to the regulator. The system automatically measures the AC voltage at both the modulated input and output. It calculates the rejection ratio as $20\text{Log}(V_{\text{in}}/V_{\text{out}})$ at each frequency within the swept band, and plots the result.

POWER 1

POWER SUPPLY REJECTION RATIO

Input Source

Ch 1

Output Source

Ch 2

Label

PSRR

Generator

Internal

External

Impedance

50 Ω

High Z

Analysis Method

Spectrum Average

Start Frequency

100 Hz

Stop Frequency

20 MHz

Sweep Profile

Auto

Custom

Constant Amplitude

100 mV


Points Per Decade

10

Go

Upon pressing Go, the oscilloscope will configure itself and the signal generator to create the desired plot based on the inputs above.

Power Supply Rejection Ratio measurement allows you to set START and STOP frequencies using the optional built-in AFG (requires 4/5/6-AFG option) or an external AFG31000 Series function generator.

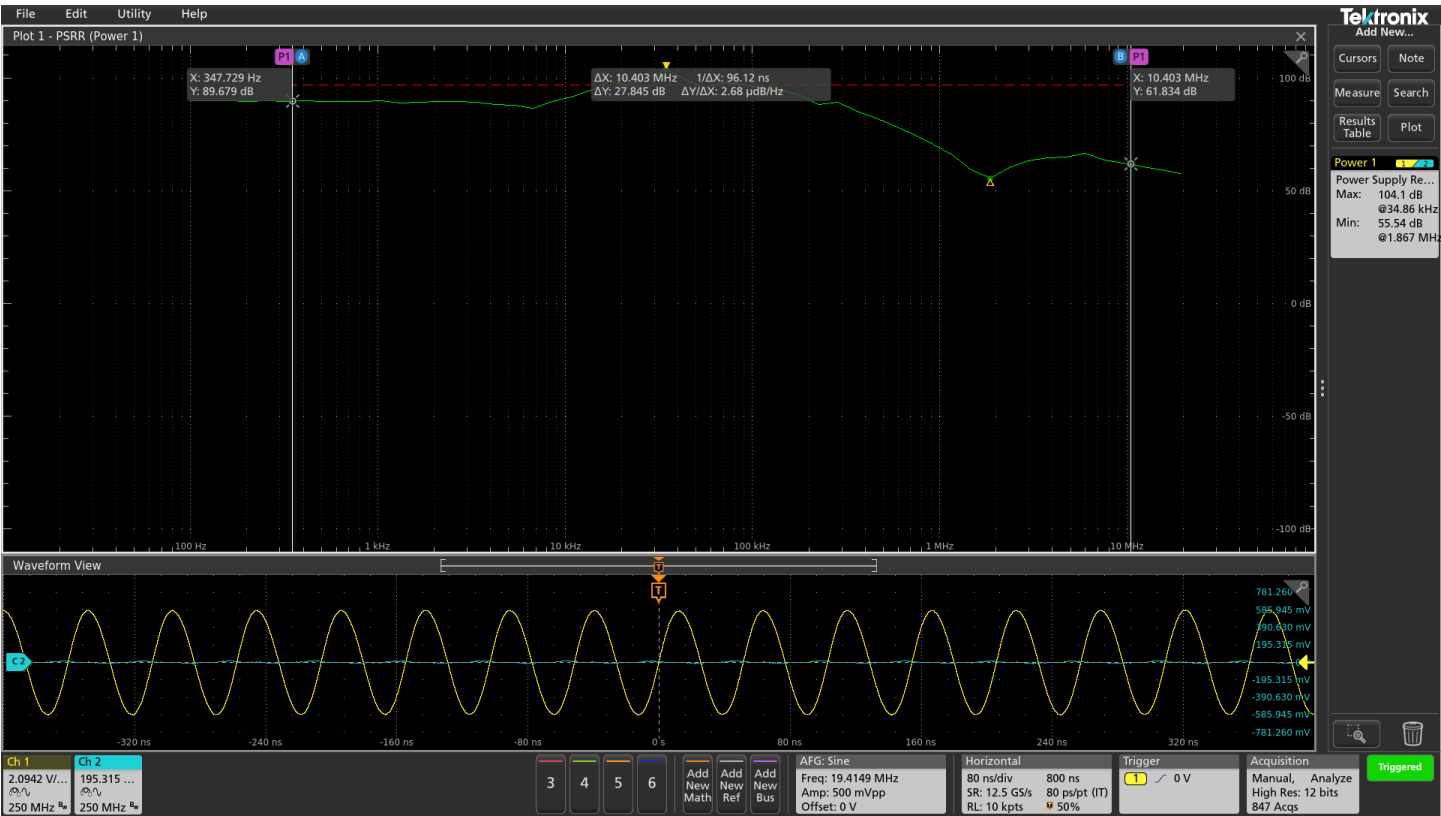

Power Supply Rejection Ratio (PSRR) plots the rejection ratio over frequencies and annotates the min and max values.

Impedance

The 2-port impedance measurement enables designers to verify the impedance of their Power Distribution Network (PDN) over a specified frequency range. The test uses the optional built-in function generator of 4/5/6 Series B MSO or an external Tektronix AFG31000 Series function generator, along with an active splitter J2161A, and power supply J2170B, an injection transformer (such as the Picotest J2102B or J2113A line injector) to measure the impedance of the PDN network. The system automatically calculates the impedance at each frequency of the swept band, and plots the results. BNC or a direct SMA connection are recommended.

POWER 1

?

IMPEDANCE

Input Source

Output Source

Label

Ch 1

Ch 2

Impedance

Splitter

Active

Passive

Generator

Internal

External

Impedance

50 Ω

High Z

Analysis Method

Start Frequency

Stop Frequency

Spectrum Average

100 Hz

20 MHz

Sweep Profile

Constant Amplitude

Points Per Decade

Auto

Custom

100 mV

10

Phase Wrap

Go

Upon pressing Go, the oscilloscope will configure itself and the signal generator to create the desired plot based on the inputs above.


Plots



Transient Response

2-port Impedance measurement allows you to set START and STOP frequencies of internal or external generator, select constant/amplitude profile, phase wrap, analysis method as spectrum view or FFT, and points per decade for better plot rendering.

Advanced Power Measurement and Analysis 4/5/6 Series B MSO Option 4-PWR, 5-PWR, and 6-PWR Application Datasheet

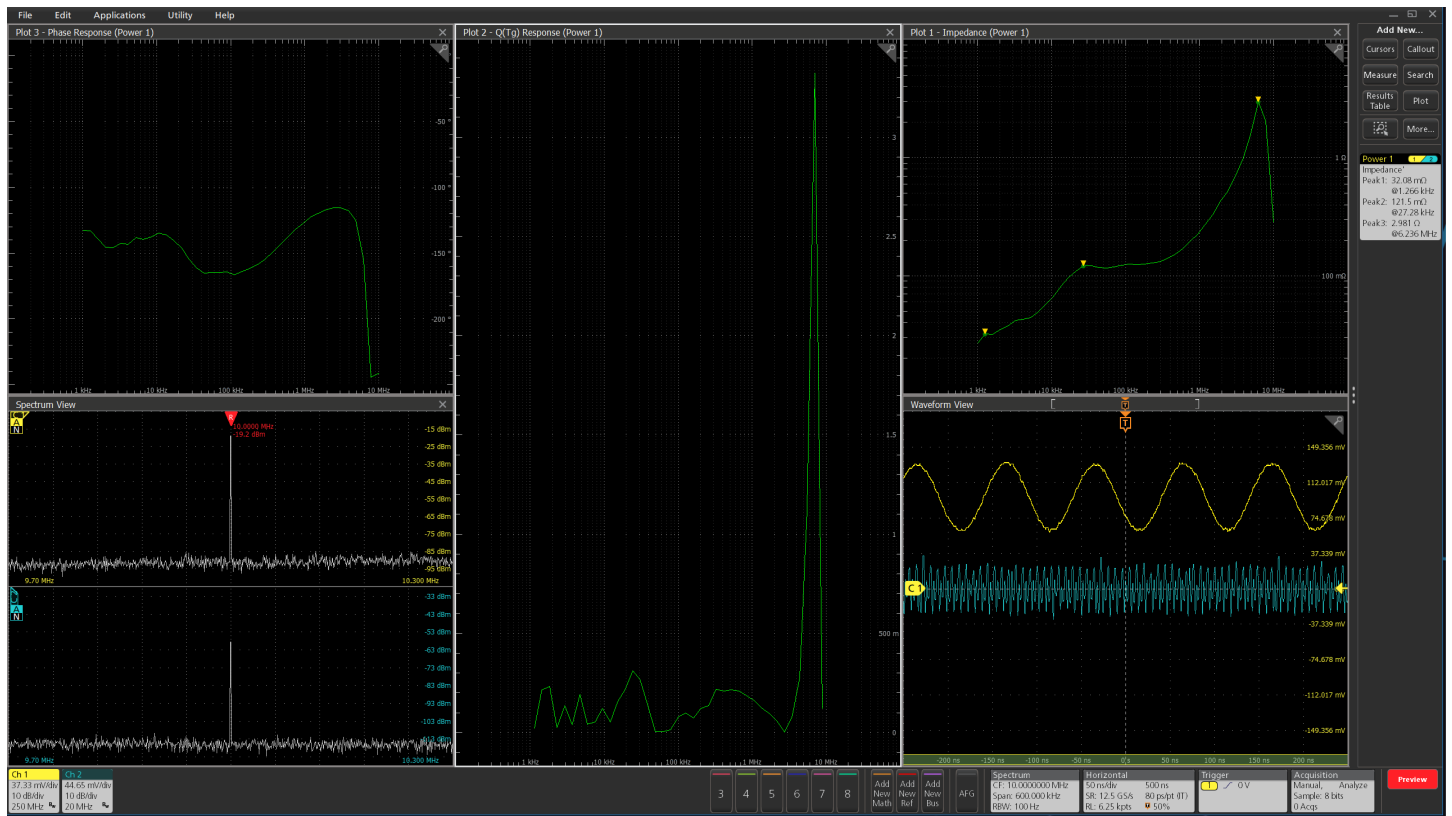

Impedance measurement with results table and results badge showing values for the peak impedance points. Corresponding impedance plot, Group Delay plot, and Phase plot are also shown.

Amplitude Profile configuration for Control Loop Response, PSRR, and Impedance Measurements

The Configure Profile menu enables precise amplitude profiling for Power Supply Rejection Ratio (PSRR), Control Loop Response (Bode), and Impedance measurements. Customize the internal or external generator's amplitude across frequency ranges to match DUT sensitivity lower amplitudes near critical crossover points and higher amplitudes elsewhere. This is beneficial especially for power supplies, which are highly sensitive near the zero-degree crossover frequency. Profiling ensures minimal distortion and optimized measurement accuracy compared to constant amplitude signals.

V_{SHUNT} measurements in power systems. For optimizing designs that use wide bandgap switching devices such as GaN or SiC transistors, IsoVu probes are unbeatable.

CONFIGURE PROFILE ?

Step	Start Frequency	Stop Frequency	Amplitude	
1	100 mHz	10 Hz	100 mV	Insert Step
2	10 Hz	100 Hz	150 mV	Delete Step
3	100 Hz	1 kHz	200 mV	Clear Table
4	1 kHz	10 kHz	250 mV	Auto Span & RBW
5	10 kHz	1 MHz	300 mV	

Configure amplitude at required start and stop frequencies. Span and RBW can be configured in spectrum view analysis method.

Smart probes deliver accurate results

Reducing noise and eliminating probing errors are among the best ways to improve the accuracy of power system measurements. The 4/5/6 Series B MSO and Advanced Power Measurement and Analysis software support a wide range of probes to help address different measurement needs, and include several features designed to help minimize probing problems.

The system uses voltage and current probes with the TekVPI interface which supports communication between probes and the scope. This allows the probe to communicate its scale setting automatically to the oscilloscope. On appropriate probes, it enables control of ranges from the front panel of the scope, and it allows probes to communicate error conditions such as a partially open jaw or a need for degaussing on current probes.

For timing-critical measurements such as switching loss, the analysis software can query voltage or current probes and use nominal delay values to remove timing skew and synchronize voltage and current waveforms for accurate and repeatable results.

The system is compatible with IsoVu Isolated Measurement Systems. These differential probing systems provide complete optical isolation, bandwidth up to 1 GHz, and extremely high common mode rejection, making them ideal for V_{GS}, V_{DS} or

Green Power Analysis


As renewable and distributed energy resources become integral to the electrical grid, inverters are required to remain connected and operate reliably during grid disturbances. Ride-through conformance testing is a critical requirement to validate this behavior and ensure compliance with evolving grid standards.

Green Power Analysis enables engineers to perform automated ride-through measurements for Distributed Energy Resources (DERs) such as photovoltaic installations, energy storage systems, wind turbines, and backup generators. These measurements help to test the ride through characteristics of the single phase grid tier inverters (GTI).

Validate inverter behavior during grid disturbances

Grid-connected inverter systems are mandated to include Anti-Islanding functionality to prevent unintended islanding during power variations on the grid. To meet these requirements, inverter performance must be verified against international standards such as CEA, IEEE1547, EVSEN50549 and Custom standards.

Tektronix provides an industry-first measurement package on its 4, 5, and 6 Series oscilloscopes to support automated ride-through conformance testing. Using Power Preset functionality, the measurement automatically set the scope settings to trigger and acquire the intermittent grid voltage disturbances and inverter voltage response behaviors during these events.

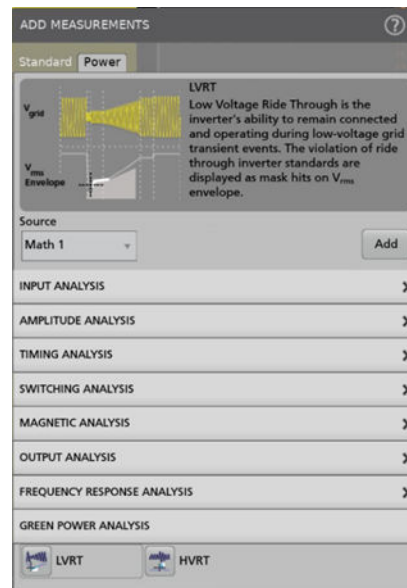


Low Voltage Ride-Through (LVRT)

LVRT is a measure of how quickly an inverter recovers from an intermittent low-voltage condition on the grid. This measurement is essential to verify that the inverter remains connected in synch with GRID and resumes normal operation within the limits defined by standards.

High Voltage Ride-Through (HVRT)

HVRT is a measure of inverter recovery behavior during intermittent high-voltage grid events. The measurement identifies whether the inverter response remains within defined voltage-time boundaries during these disturbances as per limits defined in the specifications.

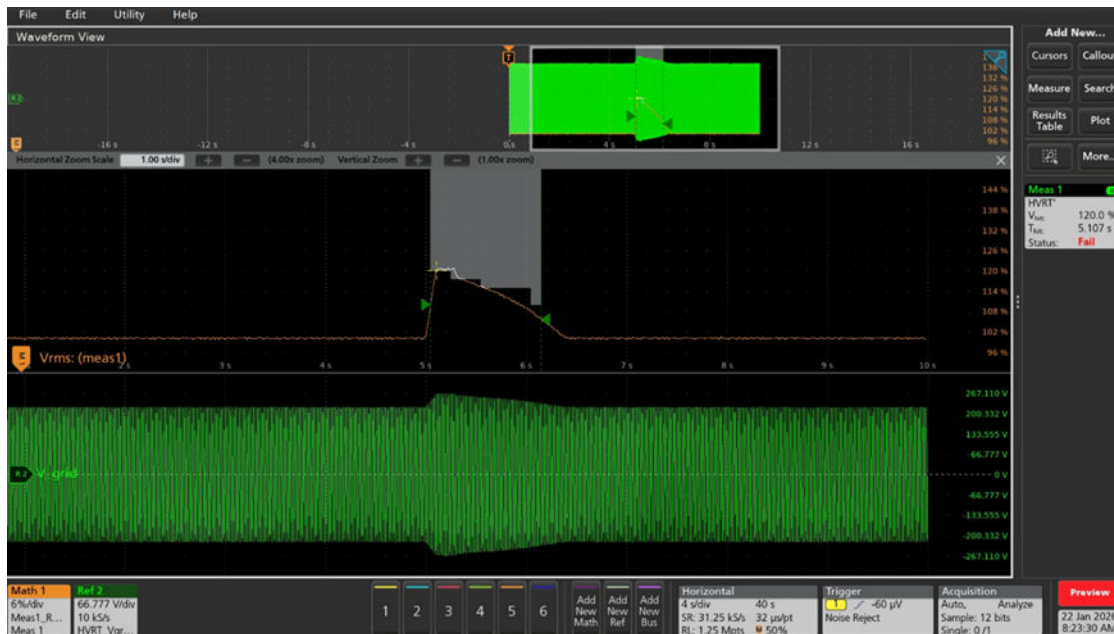

A high voltage ride-through failure, in which the RMS voltage violation on the mask.

Visualize pass/fail behavior with confidence

Ride-through results are displayed clearly against defined voltage-time masks, making it easy to identify compliance issues. The test limits are masks defined by CEA, IEEE1547-2003, IEEE1547-2018(CAT-I, CAT-II and CAT-III), EVSEN50549 CAT-I and Custom standards which define the boundary limit for recovery for the inverter RMS voltage. Any mask hits during the ride through conditions fails the test.

Automated report generation

Data collection, archiving, and documentation can be tedious, but they are critical in the design and development process. 4-PWR-BAS, 4-PWR, 5-PWR, and 6-PWR analysis software includes an automated report generator to facilitate communication and record-keeping. Press a few buttons and generate a report showing all active measurements. Add plots or append additional tests to customize your reports. Reports are available as editable .mht files, or as .pdf files. A sample report is shown below.

Power Measurements Report

Teltronix
Tuesday February 13 2018 21:51:50

Setup Configuration

Scope Details		Scope Serial Number	YaskScope Version	Scope Calibration Status
Scope Model Number		PQ200029	1.6.1	Pass

Probe Details - CH5		Probe Serial Number	Probe Cal Status
Probe Type		C022402	Default

Probe Details - CH6		Probe Serial Number	Probe Cal Status
Probe Type		B010505	Default

Power Measurement Summary Results

Power 1 - ControlLoopResponses					
Measurement	Sources	Gain Margin	Phase Cross-over frequency	Phase Margin	Gain Cross-over frequency
Control Loop Response	Ch 1, Ch 2	17.65 dB	8.791 MHz	46.20 Degrees	6.202 MHz

Power Measurement Summary Results

Power1_MagProperty									
Measurement	Sources	Peak Flux Density	Relative Flux Density	Coercive Field Strength	Maximum Field Strength	Ripple Current	Delta B	Delta H	Permeability
Magnetic Property	CH5, CH6	945.5eT	—	-2.412nAT/m	520.0nAT/m	538.8nA	799.2eT	444.4nAT/m	1.3889tm
Power1_MagLoss									
Measurement	Sources	Magnetic Loss							
Magnetic Loss	CH5, CH6	35.18mW							
Power1_VoltageV									
Measurement	Sources	1VS Integral V							
1 vs. Integral V	CH5, CH6	27.54mV/s							
Power1_Efficiency									
Measurement	Sources	Input Power	Output Power	Efficiency1	Output2 Power	Efficiency2	Total Efficiency		
Efficiency	1P: CH5, CH6 0P: CH5, CH6	35.18mW	35.18mW	100.0%	35.18mW	100.0%	200.0%		
Power1_Inductance									
Measurement	Sources	Inductance							
Inductance	CH5, CH6	1.343uH							

Power Measurement Detailed Results

Power1_MagProperty														
Measurement	Test	Sources	Mean	Min	Max	PK-PK	Std Dev	Population	Accum Mean	Accum Min	Accum Max	Accum Pk-Pk	Accum Std Dev	Accum Pop
Magnetic Property	Peak Flux Density	CH5, CH6	945.5eT	961.5eT	988.5eT	87.36eT	22.12eT	16	352.8eT	491.4eT	1.310uT	1.801uT	458.2eT	25690
Magnetic Property	Relative Flux Density	CH5, CH6	—	—	—	—	—	0	—	—	—	—	—	0
Magnetic Property	Coercive Field Strength	CH5, CH6	-2.412nAT/m	-2.412nAT/m	-2.412nAT/m	0.000AT/m	0.000AT/m	1	33.27nAT/m	359.6nAT/m	366.1nAT/m	86.51nAT/m	515	
Magnetic Property	Maximum Field Strength	CH5, CH6	520.0nAT/m	520.0nAT/m	520.0nAT/m	0.000AT/m	0.000AT/m	1	515.0nAT/m	524.3nAT/m	515.1nAT/m	41.90nAT/m	587	
Magnetic Property	Ripple Current	CH5, CH6	538.2nA	540.3nA	543.3nA	2.102nA	604.8uA	16	203.8nA	1.261nA	543.8nA	542.5nA	258.2nA	25690
Magnetic Property	Delta B	CH5, CH6	799.2eT	799.2eT	799.2eT	0.000T	0.000T	1	694.7eT	1.428eT	872.7eT	872.7eT	179.2eT	587
Magnetic Property	Delta H	CH5, CH6	444.4nAT/m	444.4nAT/m	444.4nAT/m	0.000AT/m	0.000AT/m	1	401.8nAT/m	483.8nAT/m	451.0nAT/m	450.5nAT/m	105.5nAT/m	587
Magnetic Property	Permeability	CH5, CH6	1.3889tm	1.3889tm	1.3889tm	0.000tm	0.000tm	1	1.3889tm	10.38nH/m	1.802tm	1.802tm	162.5eH/m	587

Power1_Efficiency

Measurement	Test	Sources	Mean	Min	Max	PK-PK	Std Dev	Population	Accum Mean	Accum Min	Accum Max	Accum Pk-Pk	Accum Std Dev	Accum Pop
Efficiency	Input Power	CH5, CH6	35.18mW	35.18mW	35.18mW	0.000W	0.000W	1	35.79mW	777.7uW	39.01mW	38.23mW	3.051mW	587
Efficiency	Output Power	CH5, CH6	35.18mW	35.18mW	35.18mW	0.000W	0.000W	1	35.79mW	777.7uW	39.01mW	38.23mW	3.051mW	587
Efficiency	Efficiency1	0P: CH5, CH6	100.0%	100.0%	100.0%	0.000%	0.000%	1	100.0%	100.0%	100.0%	0.000%	0.000%	587
Efficiency	Output2 Power	CH5, CH6	35.18mW	35.18mW	35.18mW	0.000W	0.000W	1	35.79mW	777.7uW	39.01mW	38.23mW	3.051mW	587
Efficiency	Efficiency2	1P: CH5, CH6	100.0%	100.0%	100.0%	0.000%	0.000%	1	100.0%	100.0%	100.0%	0.000%	0.000%	587
Efficiency	Total Efficiency	0P: CH5, CH6	200.0%	200.0%	200.0%	0.000%	0.000%	1	200.0%	200.0%	200.0%	0.000%	0.000%	587

Views

Time Domain View

Waveform View

Eff: Input Power(Power 6)

Eff: Output1 Power(Power 6)

Eff: Output2 Power(Power 6)

Δt: 49.712 μs

Δf: 79.747 μs

1/Δt: 12.54 kHz

Δw: 17.194 mW

Δw/Δt: 215.61 W/s

Δw: 7.127 mW

Δw/Δt: 15.7 μW/s

Δw: 262.830 mW

Δw/Δt: 52.5 μW/s

Plots

Plot 1 - BH Curve (Ch 5, Ch 6, Power 3)

Plot 1 - Control Loop Response (Power 1)

Plot 1 - BH Curve (Ch 5, Ch 6, Power 3)

H: 383.101 mAT/m
B: 768.777 nT
H: 174.429 mAT/m
B: 346.435 nT
ΔH: 208.672 mAT/m
ΔB: 422.342 nT
Perm: 1.46705 H/m

Plot 1 - Control Loop Response (Power 1)

Gain
Phase

Individual Measurement Configuration

Power1_MagProperty									
Voltage Source Ref Levels		Current Source Ref Levels		Configurations		Gating		General	
Global Enabled	True	Global Enabled	True	ResultCur	math2	Gating Type	None	Custom Measurement Name	Magnetic Property
Base Top Method	Automatic	Base Top Method	Automatic	ResultCurCount	Zero				
RiseHigh	90%	StartHigh	90%	Measure	St				
RiseMid	50%	RiseMid	50%	Edgesource	Voltage				
RiseLow	10%	StartLow	10%	Primarygate	1				
FallHigh	90%	FallHigh	90%	MagLength	1m				
FallMid	50%	FallMid	50%	CrossSection	1mA				
FallLow	10%	FallLow	10%						
Hysteresis	15%	Hysteresis	15%						

WWW.TEK.COM | 25

Specifications

Measurements

Measurement	Description
Input analysis	True power, Apparent power, Power factor, Reactive power, Crest factor, Phase angle, THD, Harmonics, Input capacitance, Inrush current, DO-160G, Pre-compliance testing for standard EN61000-3-2, EN61000-3-2 AM14, MIL-STD-1399 (400 Hz)
Amplitude measurements	Cycle Amplitude, Cycle Top, Cycle Base, Cycle Minimum, Cycle Maximum, Cycle Peak-to-Peak
Timing analysis	Pulse width, Duty cycle, Period, Frequency variation versus time
Switching analysis	Switching loss, Turn-on (T_{on}), Turn-off (T_{off}), Conduction loss, SOA, SOA with Mask testing, di/dt , dv/dt , $R_{DS(on)}$
Magnetic analysis	Magnetic analysis (available only in 4/5/6-PWR) Inductance, Magnetic Property, Magnetic Loss (Hysteresis Loss, Total Loss), I vs. J/V. NOTE: Not supported on option 4-PWR-BAS
Output analysis	Ripple (line frequency, switching frequency), Efficiency, Turn On Time, Turn Off Time
Frequency response analysis(available only in 4/5/6-PWR)	Bode and PSSR Control Loop Response (Bode plot) and Power Supply Rejection Ratio (PSRR). PSRR plots rejection ratio vs frequency. Control Loop Response (Bode plot) calculates gain and phase margin. Requires and recommended TPP0502, two probes. Uses the oscilloscope optional built-in generator (4/5/6-AFG required) or an external Tektronix AFG31000 Series function generator. Measurements can be made using TDP probes. Dynamic range: Bode is typically 55 dB and PSRR is typically 85 dB. Frequency: 10 Hz to 50 MHz (with option AFG). 1 Hz in case of Spectrum View method. 10 Hz to maximum sine frequency (with AFG31000 Series) Amplitude: up to 5 V (needs Option AFG or external AFG31000 Series 10V p-p). Requires Picotest isolation and injector transformers. Impedance Measurement Impedance: Requires a BNC or Direct SMA cable with DC block. Frequency: 10 Hz to 50 MHz for internal AFG and 10 Hz to max of AFG31000 Series in case of external. Minimum Impedance can be measured is 10 milli Ohm and maximum is 47 Ohms NOTE: Not supported on option 4-PWR-BAS
Green Power measurements analysis	LVRT(Low voltage ride through) and HVRT(High voltage ride through)
Plots	Time trend, Trajectory plot, Histogram, Bar graph, B-H curve, Inductance plot, I vs. $\int V$, Phase, Gain, and Rejection ratio plots.
Report	MHT and PDF format, Data export to CSV format
Degauss/Deskew (static)	Automatic detection of probes, Auto Zero. You can deskew probes from the menus for each channel

Measurement	Description
Source support	Live analog signals, reference waveforms, and math waveforms

Ordering information

Models

Product	Options	Supported instruments
New Instrument order option	4-PWR-BAS, 4-PWR, 4-PS2 5-PWR, 5-PS2, 5-PS2FRA 6-PWR, 6-PS2, 6-PS2FRA	4 Series MSO (MSO44, MSO46) 4 Series B MSO (MSO44B, MSO46B) 5 Series MSO (MSO54, MSO56, MSO58, MSO58LP) 5 Series B MSO (MSO54B, MSO56B, MSO58B)
Product upgrade option	SUP4-PWR-BAS, SUP4-PWR SUP5-PWR SUP6-PWR	6 Series MSO (MSO64) 6 Series B MSO (MSO64B, MSO66B, MSO68B)
Floating license	SUP4-PWR-BAS-FL, SUP4-PWR-FL SUP5-PWR-FL SUP6-PWR-FL	4 Series B MSO (MSO44B, MSO46B) Floating licenses are transferrable from any 4 Series oscilloscope to any other 4 Series oscilloscope, for use of one instrument at a time. 5 Series B MSO (MSO54B, MSO56B, MSO58B, MSO58LP) Floating licenses are transferrable from any 5 Series oscilloscope to any other 5 Series oscilloscope, for use of one instrument at a time. 6 Series B MSO (MSO64B, MSO66B, MSO68B) Floating licenses are transferrable from any 6 Series oscilloscope to any other 6 Series oscilloscope, for use of one instrument at a time.

Additional information about power analysis is available at <http://www.tek.com/application/power-supply-measurement-and-analysis>.

Software bundles

Bundle Options	Supported Instruments	Description
4-PRO-POWER-1Y	4 Series B MSO	1 Year License Pro Power Bundle for 4 Series B MSO
4-PRO-POWER-PER		Perpetual License Pro Power Bundle for 4 Series B MSO
4-ULTIMATE-1Y		1 Year License Ultimate Bundle for 4 Series B MSO
4-ULTIMATE-PER		Perpetual License Ultimate Bundle for 4 Series B MSO
5-PRO-POWER-1Y	5 Series B MSO	1 Year License Pro Power Bundle for 5 Series B MSO
5-PRO-POWER-PER		Perpetual License Pro Power Bundle for 5 Series B MSO
5-ULTIMATE-1Y		1 Year License Ultimate Bundle for 5 Series B MSO
5-ULTIMATE-PER		Perpetual License Ultimate Bundle for 5 Series B MSO

Bundle Options	Supported Instruments	Description
6-PRO-POWER-1Y	6 Series B MSO	1 Year License Pro Power Bundle for 6 Series B MSO
6-PRO-POWER-PER		Perpetual License Pro Power Bundle for 6 Series B MSO
6-ULTIMATE-1Y		1 Year License Ultimate Bundle for 6 Series B MSO
6-ULTIMATE-PER		Perpetual License Ultimate Bundle for 6 Series B MSO

Recommended probes and accessories

Accessory type	Recommended
Function Generator (Required for FRA if built-in AFG is not installed)	4-AFG, 5-AFG, 6-AFG instrument options
External Function Generator	AFG31000 Series
AC/DC current probes	TCP0020, TCP0030A, TCP0150
AC current probes	TRCP0300, TRCP0600, TRCP3000
Medium-voltage differential probes	TDP0500, TDP1000
High-voltage differential probes	THDP0200, THDP0100, TMDP0200
IsoVu isolated differential probes	TIVM1/L, TIVH08/L, TIVH05/L, TIVH02/L
High-voltage passive probes	P5100A, P6015A
Deskew pulse generator	TEK-DPG
Power solution bundles	4-PS2 5-PS2, 5-PS2FRA 6-PS2, 6-PS2FRA
Deskew fixture	067-1686-xx
Probes for frequency response analysis	TPP0502: Two probes for Control Loop Response, and PSSR measurements- Two BNC or Direct SMA: For Impedance measurement
Accessories for frequency response analysis	Picotest Line injector J2120A for PSRR (10 Hz to 10 MHz) Picotest Isolation transformers (for Bode) http://picotest.com : - J2100A (1 Hz to 5 MHz) - J2101A (10 Hz to 45 MHz) Picotest transformers (for Impedance): - Active Splitter: J2161A with a power supply J2170B - Common mode transformer: J2012B/J2113A for Differential Amplifier - One P2130A DC Block is needed with the BNC or SMA cable setup. - Picotest Active Splitter (J2161A)

Accessory type	Recommended
Optional external generator for frequency response analysis	AFG31000 Series Arbitrary Function Generator (FRA up to 250 MHz) AWG5200 Series and AWG70000 Series Arbitrary Waveform Generator (FRA up to 1 GHz)

Power solution bundles

4/5/6 Series B MSO PS bundle options	Description
4-PS2	4-PWR, TCP0030A, THDP0200, 067-1686-xx deskew fixture
5-PS2	5-PWR, TCP0030A, THDP0200, 067-1686-xx deskew fixture
6-PS2	6-PWR, TCP0030A, THDP0200, 067-1686-xx deskew fixture
5-PS2FRA	5-PS2, two TPP0502 probes
6-PS2FRA	6-PS2, two TPP0502 probes

Complete power probing portfolio

Use the following list of probes with option 4-PWR-BAS, 4-PWR/5-PWR/6-PWR power to ensure complete solution to power measurement capabilities on the 4/5/6 Series B MSO oscilloscopes.

Probe type	Description	
High voltage differential probes	The THDP0100/THDP0200/TMDP0200 high-voltage differential probes are the best choice for making non-ground referenced, floating measurements. These probes provide bandwidths to 200 MHz and voltage ranges up to 6000 V.	
	The P5200A/P5202A/P5205A/P5210A high-voltage differential probes are the best choice for making non-ground referenced, floating or isolated measurements. These probes provide bandwidths to 100 MHz and voltage ranges up to 5600 V.	

Probe type	Description	
Optically Isolated differential probes	The Tektronix TIVP Series IsoVu™ optically isolated differential probes are the best choice for accurately resolving high-bandwidth differential signals in presence of high common mode voltage and are ideal for testing wide bandgap designs using SiC, GaN and IGBT devices. These probes provide complete optical isolation and exceptional common-mode rejection for reliable measurements in high-voltage power systems. TIVP probes are available with 2 m and 10 m cable lengths. The TIVP1, TIVP05, and TIVP02 offer 1 GHz, 500 MHz, and 200 MHz bandwidths, respectively, and can measure differential signals up to 12500 Vpk in the presence of common-mode voltage up to 60 kV.	
Tektronix Isolated Current Probes	Designed for accurate measurement of fast-changing currents in wide-bandgap switching devices, IsoVu™ current shunt probes (TICP) provide significantly higher bandwidth up to 1 GHz compared to traditional clamp-on current probes. IsoVu isolation technology eliminates ground loops, enables safe measurements in high-voltage environments, and delivers exceptionally high common-mode rejection ratio (CMRR). These capabilities make TICP probes ideal for precision current measurements across shunts and current-viewing resistors (CVRs) in high-side SiC and GaN FET switching applications. The TICP100, TICP050, and TICP025 models offer bandwidths of 1 GHz, 500 MHz, and 250 MHz, respectively. Depending on the shunt resistor value, they support current measurements ranging from microamps to kiloamps.	

Probe type	Description	
Current probes	Tektronix offers a broad portfolio of current probes, including AC/DC current probes that provide bandwidths up to 120 MHz and best-in-class current clamp sensitivity down to 1 mA.	
	AC-only Rogowski probes include the TRCP300 (9 Hz to 30 MHz, 250 mA to 300 A peak), TRCP600 (12 Hz to 30 MHz, 500 mA to 600 A peak), and TRCP3000 (1 Hz to 16 MHz, 500 mA to 3000 A peak).	
Mid-voltage differential probes	The TDP0500/TDP1000 medium-voltage differential probes are the best choice for making non-ground referenced, floating or isolated measurements. These probes provide bandwidths to 1 GHz and voltage ranges up to ± 42 V (DC + pk AC).	
Probes for control loop analysis and power supply rejection ratio	TPP0502 is the recommended passive probe FRA measurement. It has the attenuation of 2X and bandwidth of 500 MHz. It also offers low capacity loading.	

Probe type	Description	
Probes for Impedance measurement	BNC or Direct SMA cable with DC Block are the recommended probes for Impedance measurement. The TPR1000 and TPR4000 probes provide a low-noise measurement solution (oscilloscope and probe), which is critical to not confuse the noise of the oscilloscope and probe with the noise and ripple of the measured DC supply. The higher input impedance in the probes minimizes the oscilloscope loading effect on the DC rails (50 kΩ at DC). These probes are used for Impedance testing as an alternative.	

For a complete listing of compatible probes for each oscilloscope, please refer to <http://www.tek.com/probes> for specific information on the recommended models of probes and any necessary probe adapters.

Certifications

Tektronix is registered to ISO 9001:2015 and ISO 14001:2015.

Contact Information:

Australia 1 800 709 465
Austria* 00800 2255 4835
Balkans, Israel, South Africa and other ISE Countries +41 52 675 3777
Belgium* 00800 2255 4835
Brazil +55 (11) 3530-8901
Canada 1 800 833 9200
Central East Europe / Baltics +41 52 675 3777
Central Europe / Greece +41 52 675 3777
Denmark +45 80 88 1401
Finland +41 52 675 3777
France* 00800 2255 4835
Germany* 00800 2255 4835
Hong Kong 400 820 5835
India 000 800 650 1835
Indonesia 007 803 601 5249
Italy 00800 2255 4835
Japan 81(3) 6714 3086
Luxembourg +41 52 675 3777
Malaysia 1 800 22 55835
Mexico, Central/South America and Caribbean 52 (55) 88 69 35 25
Middle East, Asia, and North Africa +41 52 675 3777
The Netherlands* 00800 2255 4835
New Zealand 0800 800 238
Norway 800 16098
People's Republic of China 400 820 5835
Philippines 1 800 1601 0077
Poland +41 52 675 3777
Portugal 80 08 12370
Republic of Korea +82 2 565 1455
Russia / CIS +7 (495) 6647564
Singapore 800 6011 473
South Africa +41 52 675 3777
Spain* 00800 2255 4835
Sweden* 00800 2255 4835
Switzerland* 00800 2255 4835
Taiwan 886 (2) 2656 6688
Thailand 1 800 011 931
United Kingdom / Ireland* 00800 2255 4835
USA 1 800 833 9200
Vietnam 12060128
*** European toll-free number. If not accessible, call:** +41 52 675 3777

Find more valuable resources at [TEK.COM](https://www.tek.com)

Tektronix®

Copyright © Tektronix. All rights reserved. Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specification and price change privileges reserved. TEKTRONIX and TEK are registered trademarks of Tektronix, Inc. All other trade names referenced are the service marks, trademarks or registered trademarks of their respective companies.

61W-61271-16 10 Sep 2026