

Dealing with a Noisy Signal: Oscilloscope Tools to Simplify Your Measurements

Introduction

Noise is a common and pervasive problem. Almost everyone involved with electrical circuits will spend some time dealing with noise - either finding its source to fix it or reducing its impact on measurements.

Noise can come from a virtually endless number of sources either internal or external to your design, obscuring your signal of interest. Perhaps you're having trouble making measurements on a low voltage (mV) signal like in a radar transmission or heart monitor. Noise can make it difficult to find the true voltage of your signal, and it can increase jitter making timing measurements difficult. Or maybe you need a clean trace free from noise to focus on the intended signal in your design. Other times, a clean trace is useful for reports and documentation to clearly show how your design works.

Your oscilloscope provides features and tools to help you deal with noise. This application note will review common oscilloscope features to reduce noise during measurements, including an innovative tool available only on the Tektronix MSO2000 and DPO2000 Series Oscilloscopes. With the FilterVu™ variable low-pass filter, you can filter unwanted noise from your signal while still capturing unexpected glitches up to the full bandwidth of the oscilloscope, enabling you to focus on your signal of interest without missing critical high-frequency events.

Using Your Oscilloscope to Measure a Noisy Signal

Stable Triggers Required

Before you analyze your signal, you need a stable display which can be a problem if your signal is noisy, making it difficult to create a stable trigger. Most oscilloscopes come with several features that assist you with this problem.

Often, the first step in creating a stable trigger is to test which trigger coupling mode works best. Many Tektronix oscilloscopes offer high-frequency (HF) reject, low-frequency (LF) reject and noise reject trigger coupling options, each of which can be used to create a stable trigger for your signal.

HF Reject performs a low-pass filter on the trigger path, attempting to ignore any high frequency instability or noise. LF Reject performs a high-pass filter on the trigger path, attempting to exclude low frequency signals from causing triggers. Noise Reject increases the required trigger hysteresis, preventing random noise from causing triggers. It may be difficult to predict how these modes will affect your particular signal; try each one, if necessary, to attain a stable trigger.

Trigger systems in most oscilloscopes also offer a holdoff control. This control only allows triggers after a user-specified delay timer. Try adjusting the holdoff to ignore some false triggers if your signal is repetitive.

If triggers are still unstable, most oscilloscopes offer a Bandwidth Limit Filter that passes the signal through a low-pass filter. The low-pass filter typically has only a few frequency settings available and often goes no lower than 20 MHz. For many applications, such as debugging power supply issues, this may not be low enough. Try the different bandwidth settings until a stable trigger is achieved.

Reducing Noise on Your Displayed Signal

Once you have a stable trigger, you can further adjust the display of noise on your oscilloscope. There are several tools available to do this: Bandwidth Limit Filter (discussed above), Average Acquisition Mode, HiRes Acquisition Mode, and FilterVu Variable Low-pass Filter, a new feature available on the Tektronix MSO/DPO2000 Series Oscilloscopes.

Bandwidth Limit Filter

The Bandwidth Limit Filter reduces the bandwidth of your oscilloscope to the frequency selected. This means that frequencies higher than the selected level will be attenuated or removed completely from the trigger path, as well as the acquisition and display path. The Bandwidth Limit Filter can be used not only for attaining a stable trigger, but also for reducing the amount of noise displayed on the oscilloscope.

Using the Bandwidth Limit Filter is one of the simplest ways to reduce noise in your oscilloscope, and works well if all the undesirable noise is at frequencies above the fixed cutoff. However, any high-speed glitches that may occur will also be removed.

Oscilloscopes typically offer a very limited set of bandwidth limit settings; standard selections include 250 MHz and 20 MHz.

Average Acquisition Mode


Average Acquisition Mode takes several complete acquisitions and averages them point by point to obtain the average voltage at each time sample in the acquisition. The number of acquisitions included in the average is adjustable by the user. Noise is typically random from acquisition to acquisition, sometimes up and sometimes down. When these random variations are averaged over enough acquisitions, they will cancel out, creating a stable signal on the screen. To utilize Average Acquisition Mode, your waveform must be repetitive. Non-repetitive waveforms or single-shot events cannot be averaged.

Average Acquisition Mode reduces all kinds of uncorrelated signals and random noise, even at very low frequencies. And, it works across all oscilloscope time/division settings.


Since multiple waveforms must be acquired to create one averaged waveform, the display can be slow to update from a changing input signal or a front-panel knob change. This means infrequent glitches will likely be missed.

In some applications, Average Acquisition Mode is a better choice than the Bandwidth Limit Filter since the full bandwidth of the oscilloscope is available to capture high frequency repetitive events.


Reducing Noise: Bandwidth Limit Filter and Average Acquisition Mode



Default acquisition and display of a small voltage sine wave. Notice the 30mV of noise on the signal.

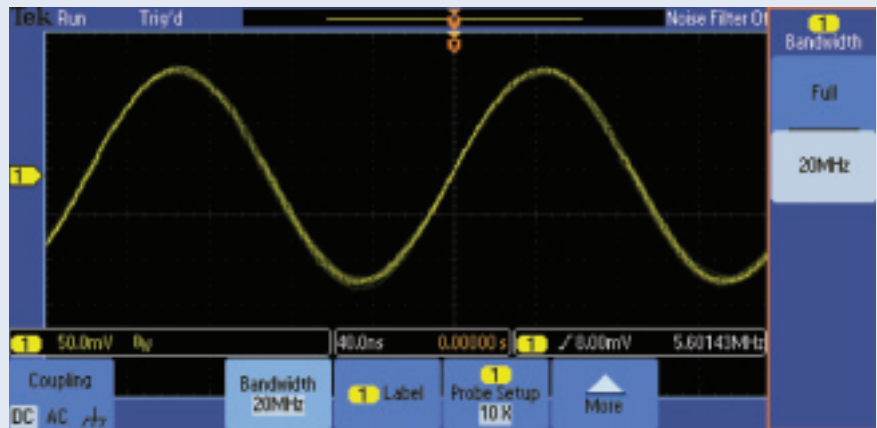

Bandwidth Limit Filter set to 20 MHz. Notice the amount of noise has been greatly reduced. This indicates that some amount of noise is greater than 20 MHz in nature, but some lower frequency noise remains.



Average Acquisition Mode with 32 averages. Notice the very clean sine wave with almost no noise. All frequencies of random noise can be removed with an average.

HiRes Acquisition Mode



Some oscilloscopes include a HiRes Acquisition Mode which is similar to Average Acquisition Mode since it uses averaging to eliminate noise. HiRes Acquisition Mode performs a box car average on each acquisition, averaging several adjacent samples within a single acquired waveform to create a single averaged sample. This has the effect of reducing high frequency noise as the average will cancel out the high speed variance in voltages caused by the noise. It also reduces the sample rate because it converts many samples into one. Therefore, HiRes Acquisition Mode is only available at slower time/division settings where the oscilloscope still has sufficient sample rate to represent the measured signal.

Unlike Average Acquisition Mode, HiRes Acquisition Mode can be used on non-repetitive and single-shot waveforms. And, since only one waveform needs to be acquired, HiRes Acquisition Mode provides a much faster update to the display after an input or front-panel setting change. The combining of neighboring samples in time also reduces the chance of aliasing at slower time/division settings.

Since HiRes Acquisition Mode is a type of low-pass filtering, you may miss high speed glitches on your signal. HiRes Acquisition Mode will pass some high frequency noise, which may obscure your signal shape and edge position. There is typically no indication of what frequencies, if any, are being removed in HiRes Acquisition Mode.

HiRes Acquisition Mode may reduce some aliased frequencies from the display; other aliased frequencies may still be present due to the poor frequency-selectivity nature of the HiRes low-pass filter.

Reducing Noise: Average and HiRes Acquisition Modes

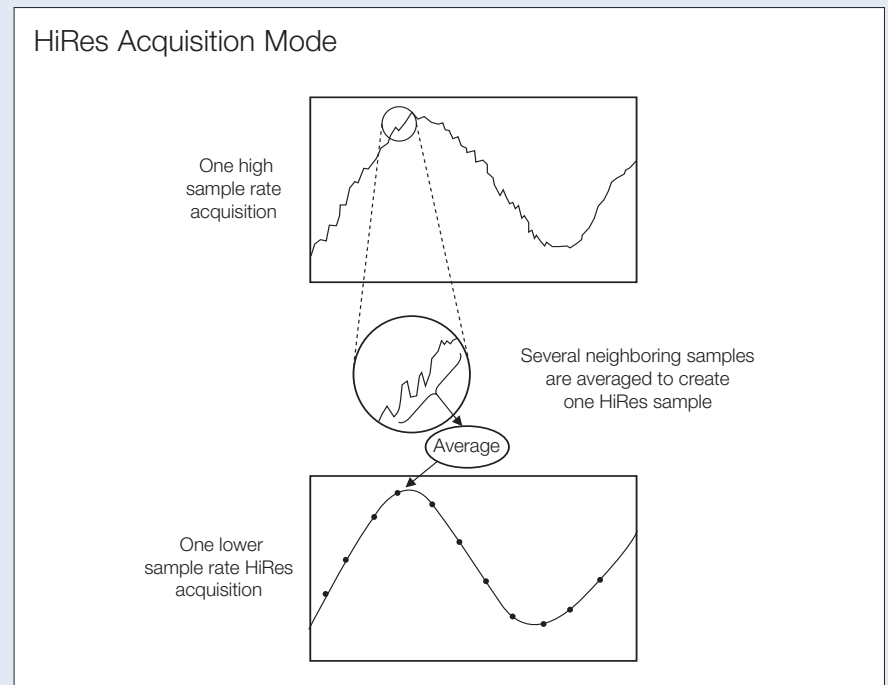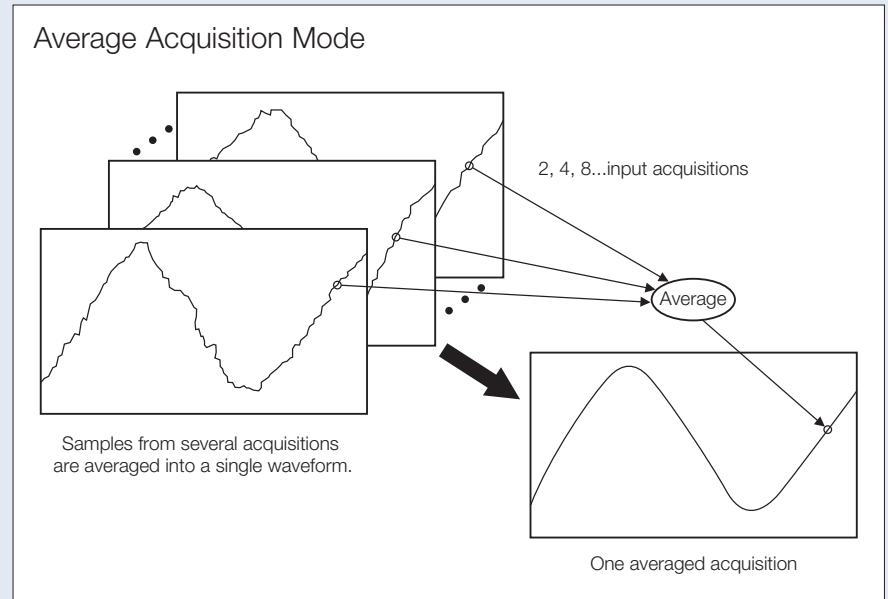

DSP Filters

Some oscilloscopes offer post-processing DSP filters which remove certain frequencies of noise from your signal. You have complete control over the filter frequency. While these filters may be flexible, they often are slow, suitable only for single-shot or slow update rate displays. They may filter out interesting and important glitches or anomalies without your knowledge.

FilterVu™ Variable Low-pass Filtering

The Tektronix MSO/DPO2000 Series Oscilloscopes offer a powerful feature, FilterVu™ variable low-pass filtering, to help filter unwanted noise from your signal. FilterVu allows you to select a low-pass filter frequency to apply to the displayed acquisition. In addition to the low-pass filtered trace, you are protected from missing any unexpected high-frequency glitches or large magnitude noise by an unobtrusive background trace showing the peak-detected (min/max sampled) raw acquisition underneath the clean filtered waveform (See Figure 1).

You can adjust the low-pass filter cutoff frequency from the front-panel, allowing you to control the amount of noise reduction you would like. Filter frequency readouts allow you to characterize what frequencies of noise are on your signal without the need to setup a cumbersome FFT (Fast Fourier Transform). This adjustment is available even on a single-shot waveform after acquisition, allowing careful inspection of your signal.

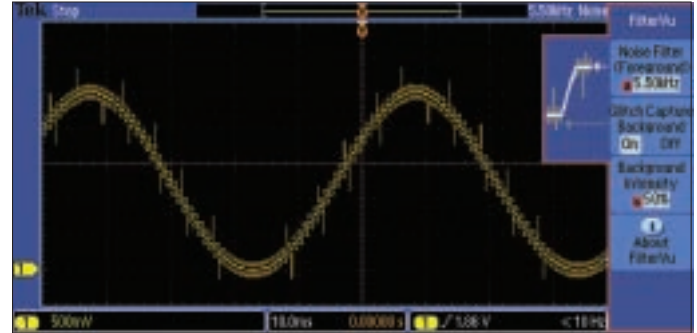


Figure 1. With the FilterVu variable low-pass filter, a background trace showing the peak-detected raw acquisition is shown underneath the clean filtered waveform.

As part of the acquisition process, FilterVu offers the fast display update of HiRes Acquisition Mode with the flexibility and control of a post-processing DSP filter, while maintaining a background image to show high-frequency glitches and noise magnitude.


The peak-detect background trace captures peak excursions of your signal up to the bandwidth of the oscilloscope, even on single-shot waveforms. This means that any glitch that can be captured at the fastest time/division setting will still be shown when inspecting your signal at the slowest time/division setting.

Just as with HiRes Acquisition Mode, FilterVu™ filtering is not available at all time/division settings. As you change to faster settings, the range of the filter is reduced. At the fastest time/division settings, no filtering is available because the low-pass filter works by reducing the number of sample points in the waveform. At many time/division settings, the oscilloscope runs at a reduced sample rate and there are many extra points. When the oscilloscope runs at or near its full sample rate, there are fewer extra points and the FilterVu functionality will be reduced. Average Acquisition Mode is the preferred choice for reducing noise at the fastest time/division settings.


FilterVu can be used on repetitive, non-repetitive, and single-shot waveforms. Its wide range of filter frequency adjustability allows you to remove just enough noise without rolling off your signal. Compared to the Bandwidth Limit Filter, FilterVu can filter to lower frequencies (less than 1 MHz), and unlike HiRes Acquisition Mode, it doesn't pass unwanted high frequencies that can obscure your signal. With its peak-detect background protecting you against missing important glitches, it is a great replacement for HiRes Acquisition Mode.

FilterVu can reduce the effects of aliasing. At the lowest available noise filter frequency at each time/division setting, no more than 1% of the high-frequency content that causes aliasing can pass through the filter when the frequency is set to the minimum, zoom is off, and acquisitions are running. Only the aliased frequencies are removed, not your signal of interest.

Reducing Noise with FilterVu™ Variable Low-Pass Filter



FilterVu capture of power-on of a switched-mode power supply. Note the small negative spike on the left of the screen. This spike is shown (circled in red) with the glitch capture feature of FilterVu. The glitch may be missed by other oscilloscopes.



This is the same single shot acquisition as the previous image with the filter frequency cutoff changed to 550 kHz. Note the oscillation on the right has now been removed from the main signal. By comparing the Noise Filter (Foreground) setting in the top right of these two examples, you can determine that the oscillation is between 550 kHz and 1.1 MHz. This analysis can be performed while stopped, all on the same single-shot capture. Note, also, that the spike is still shown in the glitch capture background. Even though you've filtered the foreground trace, the background trace is still there to show glitches.

Conclusion

Noise is a pervasive and challenging problem in nearly all electrical design and debug work. In this application note, we have discussed some of the oscilloscope tools you can use to reduce, understand, and characterize noise in your measurements. FilterVu low-pass filter in the Tektronix MSO2000 and DPO2000 Series Oscilloscopes adds a powerful and flexible tool, with fewer compromises, enabling you to better address noise issues in your designs.

Comparison of Different Filters and Acquisition Modes

Mode	Non-Repetitive and Single Shot Acquisitions	Available at Fastest Time/Division Settings	Displays High Frequency Glitches and Anomalies	Screen Update Performance	Frequency Range
Bandwidth Limit Filter	✓	✓		High	Typically only higher frequencies (20 MHz, 250 MHz)
Average Acquisition Mode		✓		Medium	N/A (all frequencies)
HiRes Acquisition Mode	✓			High	Time/division dependent
FilterVu™ Variable Low-pass Filter	✓		✓	High	Time/division dependent, user control of available filter range
DSP Filters	✓	✓		Low	Adjustable

Mode	Pros	Cons
Trigger Coupling (HF, LF, Noise Reject)	<ul style="list-style-type: none"> ■ Helps get stable trigger 	<ul style="list-style-type: none"> ■ Only effects triggering, display still noisy
Bandwidth Limit Filter	<ul style="list-style-type: none"> ■ Simple ■ Documented filter frequency ■ Helps get stable trigger 	<ul style="list-style-type: none"> ■ Limited set of filter frequencies (e.g. 20 MHz and 250 MHz) ■ Noise sources often at much lower frequencies ■ May remove important glitches
Average Acquisition Mode	<ul style="list-style-type: none"> ■ Good for repetitive waveforms ■ Available at all time/division settings ■ Adjustable – balance noise reduction with screen update performance ■ Can reduce low frequency noise 	<ul style="list-style-type: none"> ■ Doesn't work with non-repetitive or single-shot waveforms ■ Slow display response to changes in oscilloscope controls or signal changes ■ Will remove non-repeating glitches ■ Doesn't help get a stable trigger. Gives poor display results when the trigger is unstable
HiRes Acquisition Mode	<ul style="list-style-type: none"> ■ Good for repetitive, non-repetitive, and single-shot waveforms ■ Fast display update and lively input response ■ Reduces the chances of aliasing 	<ul style="list-style-type: none"> ■ Not available at fastest time/division settings ■ May remove important glitches ■ Some high frequency content not removed ■ No indication of effective bandwidth or filter frequency ■ Can't adjust filtering ■ Doesn't help get a stable trigger
FilterVu Variable Low-Pass Filter	<ul style="list-style-type: none"> ■ Adjustable filter frequency level, with a relatively wide range of filter frequencies, adjustable while running or stopped ■ Frequency readout indicates filter frequency ■ Adjustable, non-obtrusive display of glitches and noise magnitude ■ Good for repetitive, non-repetitive, and single-shot waveforms ■ Fast display update and lively input response ■ Can eliminate the chance of aliasing 	<ul style="list-style-type: none"> ■ Not available at fastest time/division settings ■ Doesn't help get a stable trigger

Contact Tektronix:

ASEAN / Australasia (65) 6356 3900
Austria +41 52 675 3777
Balkans, Israel, South Africa and other ISE Countries +41 52 675 3777
Belgium 07 81 60166
Brazil & South America (11) 40669400
Canada 1 (800) 661-5625
Central East Europe, Ukraine and the Baltics +41 52 675 3777
Central Europe & Greece +41 52 675 3777
Denmark +45 80 88 1401
Finland +41 52 675 3777
France +33 (0) 1 69 86 81 81
Germany +49 (221) 94 77 400
Hong Kong (852) 2585-6688
India (91) 80-22275577
Italy +39 (02) 25086 1
Japan 81 (3) 6714-3010
Luxembourg +44 (0) 1344 392400
Mexico, Central America & Caribbean 52 (55) 5424700
Middle East, Asia and North Africa +41 52 675 3777
The Netherlands 090 02 021797
Norway 800 16098
People's Republic of China 86 (10) 6235 1230
Poland +41 52 675 3777
Portugal 80 08 12370
Republic of Korea 82 (2) 6917-5000
Russia & CIS +7 (495) 7484900
South Africa +27 11 206 8360
Spain (+34) 901 988 054
Sweden 020 08 80371
Switzerland +41 52 675 3777
Taiwan 886 (2) 2722-9622
United Kingdom & Eire +44 (0) 1344 392400
USA 1 (800) 426-2200

For other areas contact Tektronix, Inc. at: 1 (503) 627-7111

Updated 12 November 2007

For Further Information

Tektronix maintains a comprehensive, constantly expanding collection of application notes, technical briefs and other resources to help engineers working on the cutting edge of technology. Please visit www.tektronix.com



Copyright © 2008, Tektronix. All rights reserved. Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specification and price change privileges reserved. TEKTRONIX and TEK are registered trademarks of Tektronix, Inc. All other trade names referenced are the service marks, trademarks or registered trademarks of their respective companies.
10/08 EAWOW 3GW-22049-0

Tektronix[®]

