

P7313SMA
13 GHz Differential Probe
Technical Reference



071-1968-00

P7313SMA
13 GHz Differential Probe
Technical Reference

Copyright © Tektronix. All rights reserved. Licensed software products are owned by Tektronix or its subsidiaries or suppliers, and are protected by national copyright laws and international treaty provisions.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specifications and price change privileges reserved.

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

Contacting Tektronix

Tektronix, Inc.
14200 SW Karl Braun Drive
P.O. Box 500
Beaverton, OR 97077
USA

For product information, sales, service, and technical support:

- In North America, call 1-800-833-9200.
- Worldwide, visit www.tektronix.com to find contacts in your area.

Warranty 2

Tektronix warrants that this product will be free from defects in materials and workmanship for a period of one (1) year from the date of shipment. If any such product proves defective during this warranty period, Tektronix, at its option, either will repair the defective product without charge for parts and labor, or will provide a replacement in exchange for the defective product. Parts, modules and replacement products used by Tektronix for warranty work may be new or reconditioned to like new performance. All replaced parts, modules and products become the property of Tektronix.

In order to obtain service under this warranty, Customer must notify Tektronix of the defect before the expiration of the warranty period and make suitable arrangements for the performance of service. Customer shall be responsible for packaging and shipping the defective product to the service center designated by Tektronix, with shipping charges prepaid. Tektronix shall pay for the return of the product to Customer if the shipment is to a location within the country in which the Tektronix service center is located. Customer shall be responsible for paying all shipping charges, duties, taxes, and any other charges for products returned to any other locations.

This warranty shall not apply to any defect, failure or damage caused by improper use or improper or inadequate maintenance and care. Tektronix shall not be obligated to furnish service under this warranty a) to repair damage resulting from attempts by personnel other than Tektronix representatives to install, repair or service the product; b) to repair damage resulting from improper use or connection to incompatible equipment; c) to repair any damage or malfunction caused by the use of non-Tektronix supplies; or d) to service a product that has been modified or integrated with other products when the effect of such modification or integration increases the time or difficulty of servicing the product.

THIS WARRANTY IS GIVEN BY TEKTRONIX WITH RESPECT TO THE PRODUCT IN LIEU OF ANY OTHER WARRANTIES, EXPRESS OR IMPLIED. TEKTRONIX AND ITS VENDORS DISCLAIM ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. TEKTRONIX' RESPONSIBILITY TO REPAIR OR REPLACE DEFECTIVE PRODUCTS IS THE SOLE AND EXCLUSIVE REMEDY PROVIDED TO THE CUSTOMER FOR BREACH OF THIS WARRANTY. TEKTRONIX AND ITS VENDORS WILL NOT BE LIABLE FOR ANY INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES IRRESPECTIVE OF WHETHER TEKTRONIX OR THE VENDOR HAS ADVANCE NOTICE OF THE POSSIBILITY OF SUCH DAMAGES.

Table of Contents

| | |
|---|-----|
| General Safety Summary | iii |
| Preface | v |
| Operating Basics | 1 |
| Differential Measurements for Serial Data Compliance Testing..... | 1 |
| Probe Block Diagram (Simplified) | 3 |
| Termination Voltage Control | 8 |
| Overdrive Error | 10 |
| Differential and Single-Ended Signal Measurement | 11 |
| Extending the Input Connections | 17 |
| Checking Cable Skew..... | 18 |
| Adjusting Cable Skew..... | 19 |
| Deskewing Probes | 20 |
| Reference | 23 |
| Serial Bus Standards | 23 |
| InfiniBand | 24 |
| Specifications | 25 |
| Warranted Characteristics | 25 |
| Typical Characteristics | 26 |
| Nominal Characteristics..... | 30 |
| Mechanical Characteristics | 31 |
| Performance Verification | 32 |
| Equipment Required | 32 |
| Special Adapters Required | 33 |
| Equipment Setup | 34 |
| Input Resistance | 35 |
| Termination Voltage Accuracy | 36 |
| Output Offset Zero | 39 |
| DC Gain Accuracy | 40 |
| Rise Time..... | 42 |
| Optional Accessories | 48 |
| Options | 49 |
| Maintenance | 50 |
| Inspection and Cleaning | 50 |
| Replacement Parts..... | 50 |
| Preparation for Shipment | 50 |

General Safety Summary

Review the following safety precautions to avoid injury and prevent damage to this product or any products connected to it.

To avoid potential hazards, use this product only as specified.

Only qualified personnel should perform service procedures.

While using this product, you may need to access other parts of a larger system. Read the safety sections of the other component manuals for warnings and cautions related to operating the system.

To Avoid Fire or Personal Injury

Connect and Disconnect Properly. Connect the probe output to the measurement instrument before connecting the probe to the circuit under test. Connect the probe reference lead to the circuit under test before connecting the probe input. Disconnect the probe input and the probe reference lead from the circuit under test before disconnecting the probe from the measurement instrument.

Observe All Terminal Ratings. To avoid fire or shock hazard, observe all ratings and markings on the product. Consult the product manual for further ratings information before making connections to the product.

Do Not Operate Without Covers. Do not operate this product with covers or panels removed.

Do Not Operate With Suspected Failures. If you suspect that there is damage to this product, have it inspected by qualified service personnel.

Avoid Exposed Circuitry. Do not touch exposed connections and components when power is present.

Do Not Operate in Wet/Damp Conditions.

Do Not Operate in an Explosive Atmosphere.

Keep Product Surfaces Clean and Dry.

Terms in this Manual

These terms may appear in this manual:



WARNING. *Warning statements identify conditions or practices that could result in injury or loss of life.*



CAUTION. *Caution statements identify conditions or practices that could result in damage to this product or other property.*

Symbols and Terms on the Product

These terms may appear on the product:

- DANGER indicates an injury hazard immediately accessible as you read the marking.
- WARNING indicates an injury hazard not immediately accessible as you read the marking.
- CAUTION indicates a hazard to property including the product.

The following symbols may appear on the product:



Preface

This is the technical reference manual for the P7313SMA differential probe. This manual provides operating theory, specifications, and performance verification procedures for the probe.

Operating Basics

This section discusses differential measurements using an SMA input probe for Serial Data compliance testing. It also provides information on the probe architecture and operational details to aid in its proper application.

Differential Measurements for Serial Data Compliance Testing

Differential Signaling

Gigabit serial data signals are commonly transmitted using differential signaling techniques because of improved signal fidelity and noise immunity. Although the physical layer specifications differ somewhat between the different gigabit serial data communication standards, they have some common elements. Most gigabit serial data signals are transmitted over 50 Ω transmission lines, which are terminated at both ends of a point-to-point differential interconnect. The signal transmitter provides a 50 Ω source impedance from each of its two differential outputs and the signal receiver provides an effective 50 Ω input impedance on each of its two differential inputs.

The two complementary single-ended signals that make up the differential signal are generally offset from ground at a common-mode voltage level, which allows the use of unipolar transmitters and receivers that are powered from a single power supply voltage. The transmitted signals are usually encoded using a DC-balanced encoding technique that allows the signals to be either AC or DC coupled in the transmission path. If DC coupled, the receiver termination must generally be terminated to the same DC common-mode voltage as the transmitter, to reduce DC loading on the transmitter output. An example of the single-ended signals transmitted by an InfiniBand standard driver and the resultant differential signal that would be measured by a differential measurement system is shown in *Infiniband*. (See Figure 14 on page 24.)

Although the differential response is generally the primary measurement of interest for a differential signal, full characterization of the signal also requires measurement of the single-ended response of the two complementary signals including the DC common-mode voltage.

Pseudo-Differential Measurements

A common differential measurement technique uses two single-ended probes or direct connection to two oscilloscope channels for the differential signal capture. By calculating the difference between the two input signals using waveform math, the effective differential signal seen by a differential receiver can be displayed for analysis.

This measurement technique, which is commonly referred to as pseudo-differential measurement, has a number of limitations when compared to the use of a differential probe like the P7313SMA. In addition to the obvious overhead of two oscilloscope channels for the measurement instead of the single channel needed by a differential probe, there are a number of additional problems.

Unlike the differential probe, which has been carefully designed with short, matched-input signal paths, a pseudo-differential measurement uses two oscilloscope channels, which are physically separated and generally not matched as well. Although it is possible to deskew the timing differences between two high performance oscilloscope channels to improve the accuracy of a pseudo-differential measurement, deskewing is a relatively involved procedure that may need to be repeated if any oscilloscope parameter, such as vertical gain, is changed.

The gain match between two different oscilloscope channels is also a potential problem, particularly at higher frequencies where channel gain mismatch can contribute to significantly reduced CMRR performance. The CMRR performance of a differential probe, on the other hand, is generally much better controlled, with fully characterized specifications over the full probe bandwidth.

The requirement of generating a math waveform for display of the differential signal in a pseudo-differential measurement can also introduce some subtle problems with waveform analysis, since some features such as COMM triggering or mask testing may not be fully supported with math waveforms. The use of a differential SMA-input probe like the P7313SMA also provides additional features like adjustable termination voltage that may be very useful in fully characterizing the performance of differential data transmitters. High performance oscilloscope channels are almost always limited to zero volt termination voltage, since the oscilloscope termination resistor is connected directly to signal ground.

Differential Probe Measurements

A differential probe is designed to provide a differential input interface for a single-ended oscilloscope channel. It includes a carefully matched differential signal input path and a differential buffer amplifier.

A conventional differential probe input generally has a high DC input resistance and as small an input loading capacitance as possible. The light input loading of a conventional differential probe is designed to perturb the circuit being measured as little as possible when the probe is attached.

An SMA-input probe like the P7313SMA has a very different input structure. It has a dual, matched 50 Ω input that is designed to terminate the measured signal transmission path with minimum reflections. It is designed specifically for serial compliance testing. Its SMA input connectors provide a reliable, repeatable interconnect for making accurate eye pattern measurements that are used to characterize the quality of a serial data transmission channel.

The P7313SMA probe has also been carefully designed for flat amplitude response and very small pulse response aberrations. This helps to ensure accurate eye pattern measurements over a wide data rate range.

The differential amplifier is at the heart of any device or system designed to make differential measurements. (See Figure 1.) Ideally, the differential amplifier rejects any voltage that is common to the inputs and amplifies any difference between the inputs. Voltage that is common to both inputs is often referred to as the Common-Mode Voltage (V_{CM}) and difference voltage as the Differential-Mode Voltage (V_{DM}).

The simplified input signal voltage source model driving the differential amplifier shows a complementary differential signal without source or termination impedance. In a real-world measurement, the signal source and measurement termination impedance must be known and included in the measurement analysis.

The model also shows that the output from the differential amplifier has twice the peak-to-peak amplitude of each complementary input signal.

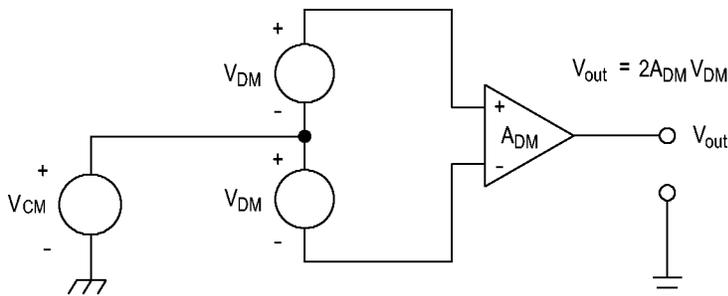


Figure 1: Simplified model of a differential amplifier

Common-Mode Rejection Ratio

Differential amplifiers cannot reject all of the common-mode signal. The ability of a differential amplifier to reject the common-mode signal is expressed as the Common-Mode Rejection Ratio (CMRR). The CMRR is the differential-mode gain (A_{DM}) divided by the common-mode gain (A_{CM}). It is expressed either as a ratio or in dB.

$$CMRR = A_{DM} \div A_{CM}$$

$$CMRR(dB) = 20 \log (A_{DM} \div A_{CM})$$

CMRR generally is highest (best) at DC and degrades with increasing frequency.

The typical CMRR response of the P7313SMA differential probe over frequency is shown in *Specifications*. (See Figure 15 on page 27.) High CMRR in a differential probe requires careful matching of the two input paths. Poorly matched signal source impedances can significantly degrade the CMRR of a measurement. Mismatches between the two differential signal input paths result in an effective conversion of V_{CM} to V_{DM} , which reduces the CMRR.

Probe Block Diagram (Simplified)

The SMA inputs and probe termination network provide a high frequency, 50 Ω signal path to the internal probe amplifier. The use of SMA-female connectors provides a reliable, repeatable attachment method for input signals. The symmetry of the input termination network is designed to reduce skew and maximize CMRR.

A simplified schematic of the P7313SMA input termination network is shown. (See Figure 2.)

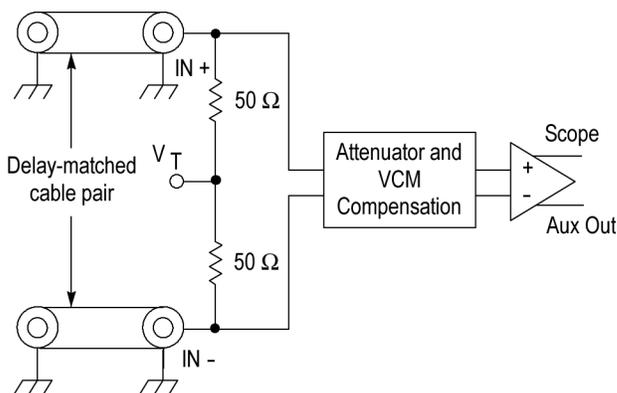


Figure 2: Input termination network

Matched-Delay Cables

The standard delay-matched cables for the P7313SMA differential probe have been carefully designed to provide guaranteed probe performance at the SMA connector interface on the end of the cable. The delay between the two matched cables in the standard cable assembly is adjusted to provide an initial skew of less than 1 ps. Cable skew this small can be degraded by cable flexure and through other environmental factors. Care should be taken to minimize physical mishandling of this quality cable assembly to preserve probe performance.

The cable used in the standard cable assembly has also been selected for its low-loss characteristics, and the cable length was selected to match the cable loss compensation designed into the probe differential amplifier. If an alternative cable assembly is used in measurements with the P7313SMA differential probe amplifier, this loss compensation characteristic must be considered. The following approximate equation for cable loss compensation can be used as a guideline in custom cable designs and is valid over a frequency range of about 1 GHz to 8 GHz:

$$Loss = -[0.5 \text{ dB} + 0.15 \text{ dB} * (F/1.25)], \text{ where } F \text{ is frequency in GHz.}$$

Custom cable pairs must also be designed with very low skew or the skew must be minimized using a pair of adjustable phase trimmer adapters like those listed in the *Optional Accessories*. (See page 48, *Optional Accessories*.)

Input Termination Network

The input termination network in the P7313SMA differential probe includes a pair of attenuation resistor networks laser trimmed to 50 Ω terminations, connected together at a common-mode voltage node, labeled V_T . (See Figure 2 on page 3.) The common-mode termination voltage node, V_T , is designed to provide a broadband, low impedance termination for input common-mode signals. The probe termination voltage can be adjusted using several different modes that will be described later.

The termination voltage range is +3.6 V/-2.5 V. For DC-coupled serial data signals, the termination voltage, V_T , should generally be set to equal the input signal common-mode voltage, V_{CM} ; for AC-coupled serial data signals, the termination voltage, V_T , should generally be set to 0 V.

The adjustability of the termination voltage also provides measurement flexibility for characterizing or stressing serial data signal drivers. Because of the low impedance of the input termination and attenuator network, the signal termination currents can become quite large. The following table can be used to calculate the DC common-mode voltages and currents at the probe inputs and termination voltage driver under several common source impedance conditions. (See Table 1.)

Table 1: Common-mode voltage and current formulas

| Common-mode term | Source impedance ¹ | |
|------------------|--|--|
| | 0 Ω | 50 Ω |
| V_I | V_{CM} | $0.5 \times (V_T + V_{CM})$ |
| I_I | $40.00 \text{ mA} \times V_T - 40.00 \text{ mA} \times V_{CM}$ | $20.00 \text{ mA} \times V_T - 20.00 \text{ mA} \times V_{CM}$ |
| I_T | $40.00 \text{ mA} \times V_T - 23.33 \text{ mA} \times V_{CM}$ | $28.33 \text{ mA} \times V_T - 11.67 \text{ mA} \times V_{CM}$ |

¹ When inputs are AC coupled: $V_I = V_T$, $I_I = 0$, $I_T = 16.67 \text{ mA} \times V_T$

The probe block diagram shows that the input termination network is followed by an attenuator and V_{CM} compensation circuit. The attenuator is used to increase the effective input dynamic range of the probe differential amplifier.

The P7313SMA probe has two attenuation settings, 2.5X and 12.5X, that allow dynamic range to be traded off against signal noise. The 12.5X attenuator setting has the largest dynamic range; the 2.5X attenuator setting has the lowest noise.

The V_{CM} compensation circuit automatically minimizes the DC common-mode voltage at the probe differential amplifier inputs even with varying termination voltage and input signal DC common-mode voltage. This maximizes the differential mode signal input dynamic range. The V_{CM} compensation circuit allows the DC common-mode input voltage range to be the same for both attenuator settings. (See Figure 4 on page 7.)

Internal Probe Amplifier

The P7313SMA differential probe is designed to measure high frequency, low-voltage circuits. Before connecting the probe to your circuit, take into account the limits for maximum input voltage, the common-mode signal range, and the differential-mode signal range. For specific limits of these parameters, see the *Specifications* section. (See page 25, *Specifications*.)

Maximum Input Voltage. The maximum input voltage is the maximum voltage to ground that the inputs can withstand without damaging the probe input circuitry.




CAUTION. To avoid damaging the inputs of the P7313SMA differential probe, do not apply more than ± 5 V (DC + peak AC) between each input and ground. In addition, to avoid probe damage, the maximum termination resistor power must not be exceeded.

Maximum Termination Resistor Power. The internal termination resistors can safely dissipate 0.2 W of power continuously, which is the case for normal probe operation without termination driver current overload. However, the probe will be damaged if you apply more than 0.5 W of power through the termination resistors for more than 5 minutes.

If you suspect your measurement application will approach these limits, use the formulas that follow to calculate the power dissipated by the termination resistors.

The power calculation formulas are based on the simplified model, which represents the signal at the probe inputs. (See Figure 3 on page 6.) If a signal source with 50 Ω source impedances is used, the signal levels used should match the zero-ohm source impedance model shown in the figure.

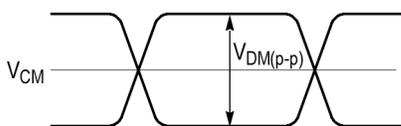

$$\text{DC power} = \left[\frac{V_{CM} - V_T}{50} \right] (V_{CM} - V_T) \text{ per side}$$

$$\text{AC power} = \left[\frac{V_{DM(p-p)}}{100} \right] \left[\frac{V_{DM(p-p)}}{2} \right] \text{ per side}$$

The signal source model defined for these equations is as follows:

V_+ and V_- = Single – ended signals into a 50 Ω load

$$V_+ = V_{CM} + V_{DM} \quad V_- = V_{CM} - V_{DM}$$

This results in the terms to be used in the preceding power equations:

$$V_{CM} = (V_+ + V_-) \div 2 \quad V_{DM} = (V_+ - V_-) \div 2$$

V_T = Termination input voltage

NOTE. With a balanced DC signal, in the preceding equations, V_{DM} is half of the value of a conventional differential signal.

$$V_{Diff} = V_+ - V_- = 2V_{DM}$$

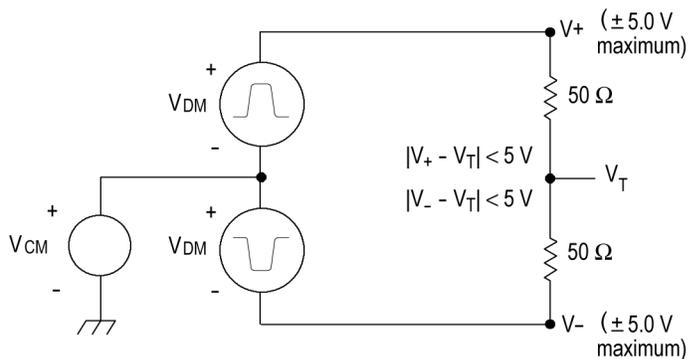


Figure 3: Probe maximum input limits

Common-Mode Signal Range. The common-mode signal range is the maximum voltage that you can apply to each input, with respect to earth ground, without saturating the input circuitry of the probe. A common-mode voltage that exceeds the common-mode signal range may produce an erroneous output waveform even when the differential-mode specification is met.

Differential-Mode Signal Range. The differential-mode signal range is the maximum voltage difference between the plus and minus inputs that the probe can accept without distorting the signal. The distortion from a voltage that is too large can result in a clipped or otherwise distorted and inaccurate measurement. The differential mode signal range is dependent on the probe attenuator setting as shown. (See Figure 4.)

For a more detailed description of the differential mode dynamic range, see *Differential Measurement Topology*.

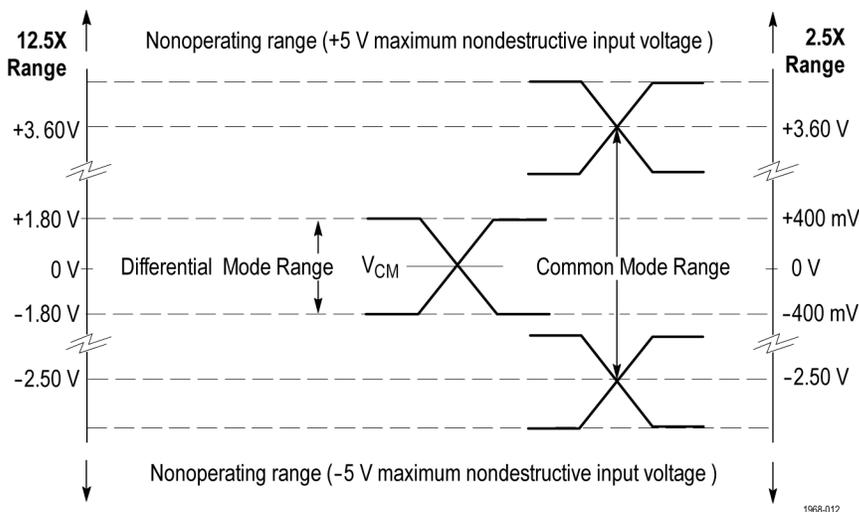


Figure 4: Differential and Common-Mode operating ranges

Common-Mode Rejection. The common-mode rejection ratio (CMRR) is the ability of a probe to reject signals that are common to both inputs. More precisely, CMRR is the ratio of the differential-mode gain to the common-mode gain. The higher the ratio, the greater the ability to reject common-mode signals.

Probe Amplifier Outputs. The P7313SMA probe has a differential signal output. The positive polarity output is connected to the oscilloscope through the TekConnect probe interface. The inverted polarity output is connected to the Aux Output SMA connector on the top of the probe.

The positive polarity main output is automatically scaled by the intelligent TekConnect probe interface to compensate for probe attenuation and display the differential signal voltage at the probe inputs. The inverted Aux Output is an attenuated version of the differential signal input, which must be manually accounted for in signal measurements or processing.

Termination Voltage Control

The P7313SMA probe termination voltage can be controlled either internally or externally, as selected by three different modes. A block diagram of the probe termination network is shown. (See Figure 5.) A discussion of the circuitry follows.

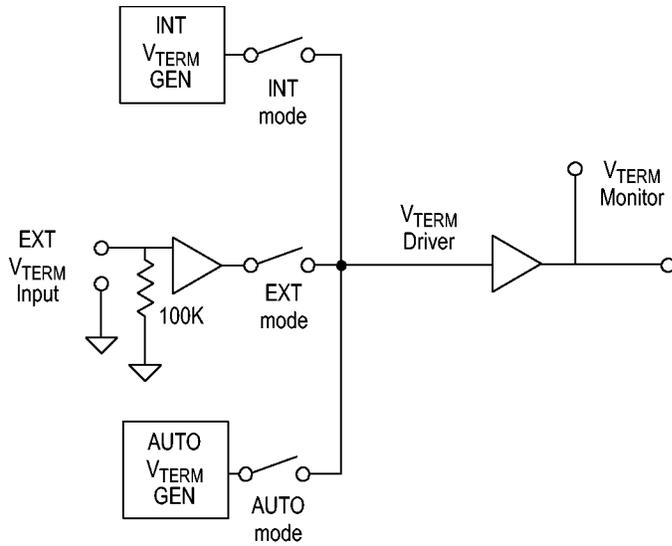


Figure 5: Termination voltage network drive

The P7313SMA probe is designed for compliance testing of high-speed, serial data standards such as PCI Express, InfiniBand, SerialATA, XAUI, Gigabit Ethernet, Fibre Channel, and others. All of these high-speed, differential data standards define a common-mode voltage less than the +3.6 V/-2.5 V termination range of the P7313SMA probe.

The probe termination voltage can be set to the desired input signal common-mode voltage using one of three control modes: Auto (the default mode at power-on), Internal, and External. The operation of these modes are described below.

Auto Mode

When the probe is first connected to the oscilloscope, a self test runs, and the default termination voltage control mode is set to Auto. When the probe is in Auto mode, the common-mode voltage of the input signal is monitored, and the DC termination voltage is set to match the common-mode input voltage. Auto mode provides the minimum DC loading on the input signal source.

With open inputs or a high DC source impedance, such as an AC-coupled input signal, the Auto mode select LED flashes, indicating that the termination voltage has been set to zero volts.

This is the mode that you will likely use for most compliance testing of current serial data standards.

Internal (Int) Mode

The internal mode allows you to set the termination voltage with user controls that are available on some TekConnect-interface oscilloscopes. You can adjust the DC termination voltage within the +3.6 V/-2.5 V range. See your oscilloscope manual for details on using this mode.

External (Ext) Mode

When the probe is in external mode, it allows control of the DC termination voltage with an external power supply. You can adjust the DC termination voltage within the +3.6 V/-2.5 V termination voltage range of the probe.

The external DC termination voltage control input is buffered by an internal amplifier with 100 K Ω input impedance.



WARNING. Do not exceed the ± 15 V maximum external mode voltage for the probe. Excess voltage will damage the probe.

In Ext mode, the external DC voltage is connected to the red (+) and black (-) terminals on the end of the probe head, which accept standard 80 mm plugs. A pair of 0.080 in-to-banana plug adapter cables are included with the probe for making connections from these connectors to external power sources. The black terminal is ground and is connected to the outer case of the shielded module that holds the SMA input terminals. When you are not using these terminals, they can be left open and unconnected. When the Ext mode input terminals are left open, the Ext mode termination voltage defaults to 0.0 V.

The termination voltage supplied to the input termination network by the Vterm driver can be monitored with a DMM on a pair of 0.040 inch pin jacks on the top of the probe. This allows you to verify the termination voltage setting, and when you are using Auto mode, allows you to measure the common-mode input voltage.

You can use a pair of 0.040 inch-to-0.080 inch pin jack adapters with the 0.080 inch-to-banana plug cables (both are standard accessories included with your probe), to make a more permanent connection to the monitoring DMM.

Overdrive Error

The P7313SMA differential probe can measure signals that have a common-mode voltage range of ± 2.5 V. Although the termination voltage range is specified to be +3.6 V/-2.5 V, limitations on the linear current range of the termination voltage driver restrict the voltage difference between V_{CM} and V_T .

Generally, you must keep the termination voltage within about 2 volts of the common-mode voltage (when using a supply with 0 Ω source impedance), or 3 volts of the common-mode voltage (with a 50 Ω source impedance), or the Overdrive Error LED will glow solid, indicating an over-current situation, which may lead to a measurement error.

The specific voltage difference between V_{CM} and V_T is dependent on both the source impedance and the V_{CM} and V_T values. You can use the input termination network table to determine allowable conditions, with the Overdrive Error current threshold for I_T set at about ± 80 mA. (See Table 1 on page 4.)

The Overdrive Error LED will also flash red when the termination voltage exceeds the allowable +3.6 V/-2.5 volt range. This can occur in Auto mode when V_{CM} exceeds a threshold of about ± 2.8 V, or in Ext mode when the V_T input voltage exceeds the same threshold. If this occurs, remove all signal sources from the probe to clear this LED.

The Overdrive Error LED provides an active status monitor of error conditions; it does not latch and store the occurrence of an error condition.

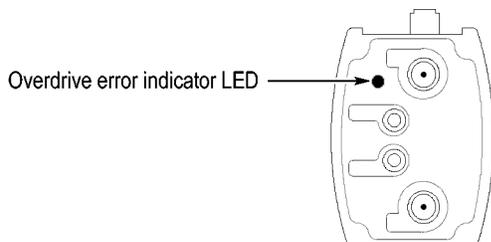


Figure 6: Overdrive Error indicator

Differential and Single-Ended Signal Measurement

Although designed for differential signal measurement, the P7313SMA probe can be used to make single-ended measurements when properly configured. The analysis that follows describes some differential and single-ended measurements of typical high-speed serial data signals.

Differential Measurement Topology

A typical differential measurement topology using the P7313SMA probe is shown. (See Figure 7.) The termination network for the probe in this figure includes a termination capacitor. This is intended to show that the termination network provides a broadband AC ground for common-mode signals.

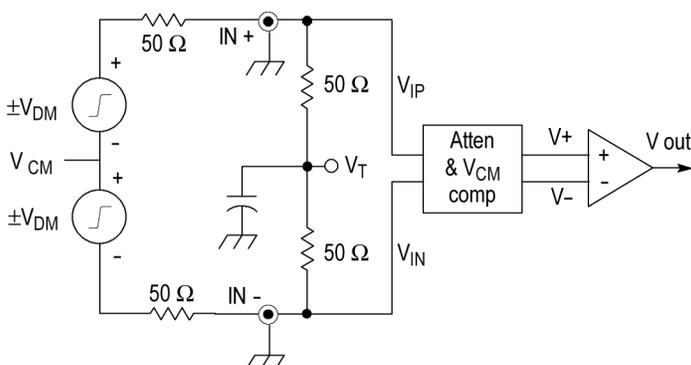


Figure 7: Differential measurement topology

Although an ideal differential signal is theoretically terminated at the V_T node due to symmetry, the low impedance V_T node terminates any non-ideal, AC common-mode signal components. The input signal source model includes a common-mode component, V_{CM} , and complementary differential mode components, $\pm V_{DM}$.

The differential mode signal source models have double the signal amplitude of the measured signal at each input because of the 50 Ω voltage divider between the source and termination resistance. The common-mode signal source model does not have double the signal source amplitude because most serial data transmitters are designed to drive a load resistance terminated with the DC common-mode voltage, not signal ground.

With V_T set equal to V_{CM} in this model topology, the DC common-mode voltage at each probe input should equal V_{CM} . The resulting differential signals at the probe inputs are:

$$V_{IP} = V_{CM} + V_{DM} \quad V_{IN} = V_{CM} - V_{DM}$$

The attenuator and V_{CM} compensation network that follows the termination network nulls out the V_{CM} signal and attenuates the V_{DM} signals. The resulting differential signals at the probe amplifier inputs for a 2.5X attenuation setting are:

$$V_+ = 0.4V_{DM} \quad V_- = -0.4V_{DM}$$

The resulting output signal from the probe output is:

$$V_{out} = -0.8V_{DM}$$

The inverted polarity of the probe amplifier output can be verified by examining the probe Aux Output signal. The main probe output signal is routed through the TekConnect interface connector and is automatically scaled to show the correct differential amplitude at the probe input connectors.

Differential Dynamic Range

The V_{CM} compensation circuit in the probe attenuator is designed to maximize the dynamic range of the AC component of the input signal. For most high-speed serial data signals, the AC component of the signal is of most interest for compliance testing where an eye pattern display of the differential signal is checked for timing jitter and voltage amplitude and fidelity.

The DC common-mode component of the input signal is present primarily to bias the signal into the operating range of the receiver and may even be removed in the transmission path with AC coupling. The V_{CM} compensation circuit in the P7313SMA probe is designed to null out the DC common-mode component of the input signal, V_{CM} , so that only the differential mode component of the input signal is passed through to the probe amplifier inputs.

The V_{CM} compensation circuit allows the dynamic range of the probe to be specified as a differential peak-to-peak voltage with a separate DC common-mode range. The differential peak-to-peak voltage specification is different for the two probe attenuation settings, but the DC common-mode range is the same for both attenuation settings.

The DC common-mode range of the probe is actually describing the performance of the V_{CM} compensation circuit, rather than the dynamic range of the probe amplifier. The dynamic range of the probe has been specified as a differential peak-to-peak voltage because that best represents the way in which the signal is typically displayed and specified for compliance testing.

Single-Ended Measurement Topology

Although the P7313SMA differential probe can be used to make single-ended measurements, it is important to understand the impact of the termination network on the measured response, particularly on the DC common-mode component of the signal.

Because of the limited dynamic range of the probe amplifier, single-ended measurements, which also display the DC common-mode component of the signal, must be carefully checked for possible overdrive problems. The single-ended measurement topology can also affect the performance of Auto mode, which will only function properly with a matched source impedance configuration.

Three possible single-ended measurement topologies will be examined in this section. They differ in the termination used on the (-) input of the probe when the single-ended signal is connected to the (+) input.

50 Ohm Termination on (-) Input. A single-ended measurement topology with a 50 Ω termination on the probe (-) input is shown. (See Figure 8.) The general equations that describe the response of that topology are also shown, including DC loading on the signal source.

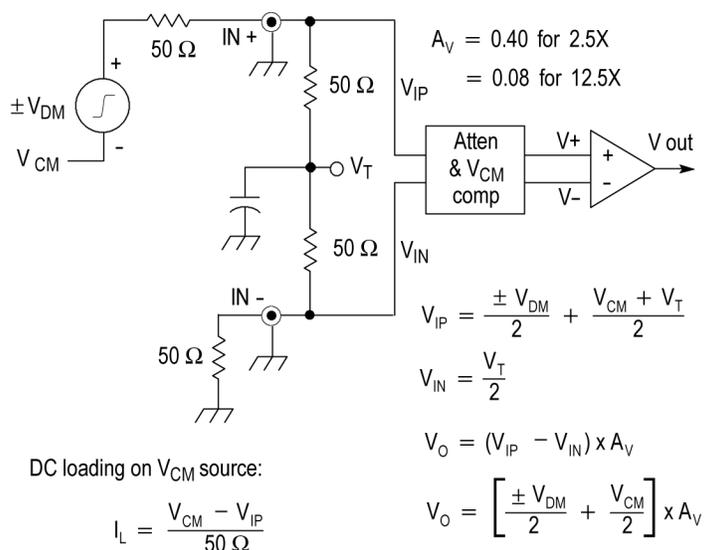


Figure 8: 50 ohm termination on (-) input

The equations for this topology show that varying the termination voltage, V_T , affects the DC loading on the signal source, but does not affect the measured DC voltage. The measured, single-ended DC voltage also represents only half the common-mode input voltage, V_{CM} , because of the voltage divider network formed by the four 50 Ω resistors and the differential amplifier response.

Although the 50 Ω termination resistors have been laser trimmed for guaranteed performance, it should be noted that the precision of the signal measurement in this topology is affected by the signal source impedance and the impedance of the 50 Ω termination resistor inside the probe positive input connector. This matched source impedance topology is the only single-ended topology that can be correctly used with Auto mode.

Shorting Termination on (-) Input. An alternative single-ended measurement topology with a shorting termination on the (-) input is shown. (See Figure 9.) The general equations describing the response and loading of this topology are also shown. The equations for this topology show identical loading of the signal source when compared to the 50 Ω termination topology. This is because the termination voltage, V_T , effectively isolates input signal loading from the termination on the probe negative input.

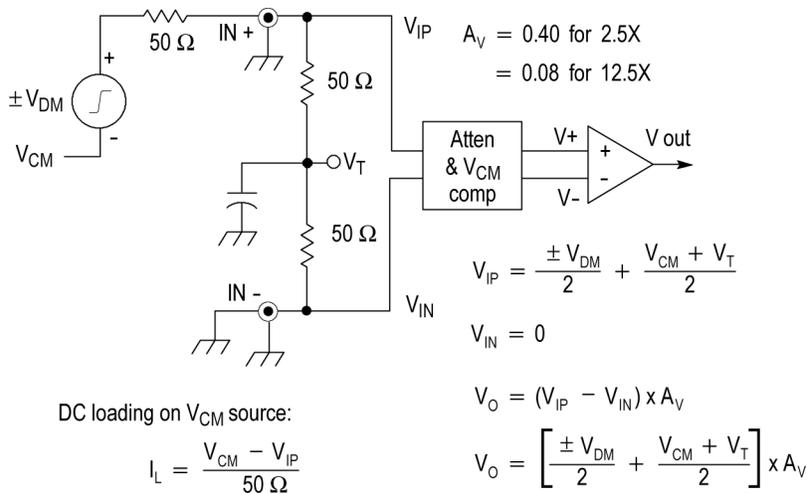


Figure 9: Shorting termination on (-) input

The measured single-ended signal response for this topology differs from the 50 Ω termination topology. The measured AC voltage, V_{DM} , is the same for both single-ended topologies, but the measured DC voltage is affected by both the common-mode input voltage, V_{CM} , and the termination voltage, V_T .

In the special case where the termination voltage is set equal to the common-mode input voltage, the input signal DC loading is minimized and the measured DC output voltage equals the full common-mode input voltage, scaled by the probe attenuation. The intelligent TekConnect probe interface automatically accounts for the probe attenuation setting and a TekConnect oscilloscope will display the full single-ended input signal when V_T equals V_{CM} .

Although this topology displays the correct DC common-mode voltage, it also has a greater risk of exceeding the probe dynamic range and overdriving the probe amplifier.

Open (-) Input. Another alternative single-ended measurement topology is shown. (See Figure 10.) In this case, the (-) input is left open, effectively keeping it at the V_T voltage level. The general equations describing the response and loading of this topology are also shown.

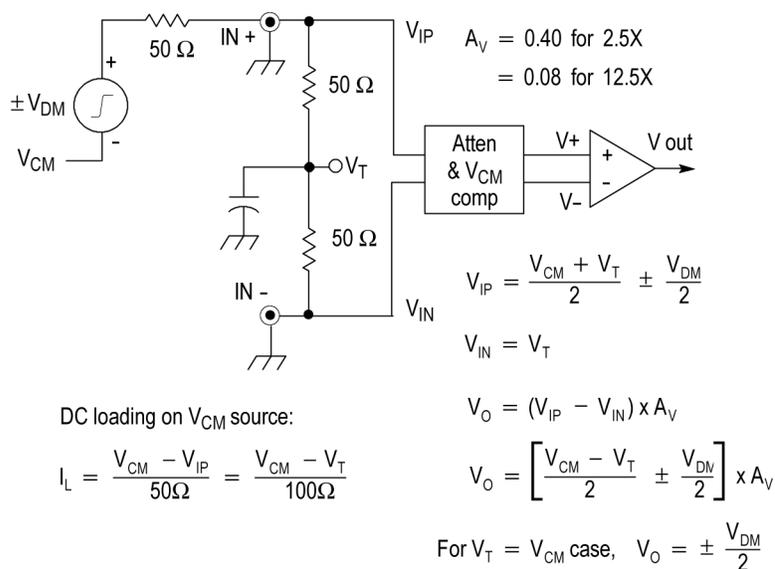


Figure 10: Open (-) input

The measured single-ended response for this topology has the same AC voltage, V_{DM} , as the other topologies, but has a common-mode voltage term that is proportional to the difference between V_{CM} and the termination voltage, V_T . In the special but common case, where $V_T = V_{CM}$, only the AC component is displayed, somewhat like an AC-coupled condition.

Single-Ended Measurement Procedure

The description of characteristics of the three alternative single-ended measurement topologies suggests the following procedure for making single-ended measurements on serial data signals that require light DC loading, (for example, when $V_T = V_{CM}$):

First, determine the common-mode input voltage, V_{CM} , of the single-ended signal by making a measurement with the 50 Ω termination topology shown. (See Figure 8 on page 13.) With this topology and the Termination Voltage Select set to Auto mode, the common-mode input voltage can be measured with a DMM on the Termination Voltage Monitor output pins.

Note that measuring the common-mode input voltage on the single-ended signal using this topology is more accurate than using a differential measurement topology, where the measured common-mode voltage is the average between the two single-ended signals that comprise the differential signal. The common-mode voltage for each of the single-ended inputs that comprise the differential signal should be measured independently and recorded for use in the second step of this procedure.

Next, since the 50 Ω termination topology only displays half the common-mode input voltage, it is now necessary to switch to the shorting termination topology shown. (See Figure 9 on page 14.) This can be done simply by changing the termination attached to the (-) input from a 50 Ω SMA termination to an SMA shorting termination.

Since Auto mode only works with matched-source impedances on both probe inputs, it is also necessary to switch the Termination Voltage Select to either Int or Ext mode. The termination voltage should be set to the voltage measured in the first step. This can be done easily in Int mode, but requires a TekConnect oscilloscope that has support for probe termination voltage select.

Setting the termination voltage in Ext mode requires the use of an external power supply and the accessory cables supplied with the probe. Once the termination voltage has been set to match the DC common-mode input voltage, the complete input signal is displayed with the shorting termination topology. This shorting termination topology, however, has the highest risk of exceeding the probe dynamic range. Dynamic range calculations for single-ended measurements will now be described.

Single-Ended Dynamic Range

The dynamic range of the probe has been specified for differential measurements, as described in the differential measurement topology section. When single-ended measurements are made, the input common-mode voltage is no longer nulled out, but becomes a differential mode DC signal that must be within the input dynamic range of the probe to be measured accurately.

The specified dynamic range for differential signals, which is expressed as a differential peak-to-peak voltage, can be converted to a more conventional voltage range for single-ended signal measurements as shown. (See Table 2.)

Table 2: Differential to single-ended conversion table

| Attenuation | Differential measurement dynamic range | Single-ended measurement dynamic range |
|-------------|--|--|
| 2.5X | 800 mVp-p | ± 0.400 V |
| 12.5X | 3.6 Vp-p | ± 1.8 V |

Because the common-mode DC voltage of many serial data signals is larger than the signal differential mode voltage, the relatively small single-ended dynamic range in the 2.5X attenuation setting may not be adequate. As a result, single-ended measurements will generally be made using the 12.5X attenuation setting.

In the case where single-ended measurements are made on signals with a large common-mode DC voltage, it should be noted that the use of the 50 Ω termination topology effectively attenuates the DC common-mode voltage by half. If this is taken into account as an offset to the displayed signal, it allows single-ended signals with a relatively large DC common-mode voltage to be measured.

If only the AC component of the single-ended signal needs to be measured, then the open input topology provides the greatest dynamic range.

Although it is possible to attenuate an input signal with external attenuators to increase the effective dynamic range, care should be taken to account for the signal loading and the impact on the termination voltage of the probe.

If an external attenuator is used, its attenuation accuracy must be taken into account when factoring the impact on measurement accuracy. The increase in attenuation also brings an increase in noise.

Extending the Input Connections

At times it may be necessary to extend the probe inputs with cables that are longer than the standard 38 inch cables. The 38 inch cables are precision-matched to minimize time-delay differences (skew).

If you substitute cables, you should use low-loss, flexible cables and keep the lengths matched and as short as possible to minimize skew and optimize common-mode rejection. Check the skew between the cables, and if necessary, use a pair of phase adjusters to minimize the skew.

Extending the input leads will also increase the skin loss and dielectric loss, which may result in distorted high-frequency pulse edges. You must take into account any effects caused by the extended leads when you take a measurement.

Checking Cable Skew

The time-delay difference (skew) between the ends of the matched-delay SMA cable pair supplied with the probe is typically less than 1 ps. If you use a pair of matched, high-quality, low-loss cables other than those supplied with the probe, you can bring the skew to within 1 ps by using a pair of phase adjusters. (See page 48, *Optional Accessories*.)

You can measure the skew of a pair of matched cables by connecting the cables to a Tektronix 80E08 or 80E10 Sampling Head, configured for a TDR output. (See Figure 11.)

1. Turn on the equipment and let it warm up for 20 minutes. Do not connect the cables to the sampling head yet.
2. Do a system compensation for the TDR module, and then verify the skew of the two outputs with the TDR outputs open, using a common-mode TDR drive.

Skew between the two outputs can be compensated with the TDR module deskew control. Refer to your sampling head or oscilloscope manual for instructions.

3. Connect the matched cable pair to the TDR outputs.

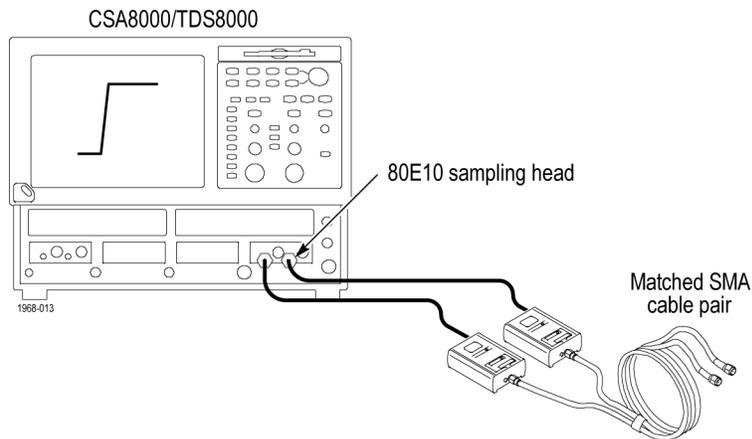


Figure 11: Checking skew between inputs

4. The measured skew of the matched cable pair that are supplied with the probe should be less than 1 ps. User-supplied cables may not be nearly as accurate, and may require some trial-and-error testing to select an optimally-matched pair. Adjust the horizontal scale to locate the pulse (to account for the cable delay; it is approximately 4.5 ns for the cable set supplied with the probe). If you use the system cursors, be aware that the displayed time is the round-trip time (step and reflection). You need to divide the displayed time difference by 2 to derive the actual skew.

If you need to minimize the skew of a pair of cables not supplied with the probe, continue with *Adjusting Cable Skew*. (See page 19, *Adjusting Cable Skew*.)


Adjusting Cable Skew

If you want to minimize the skew introduced by cable pairs other than those supplied with the probe, you can use a pair of phase adjusters to bring the skew to within 1 ps. (See page 48, *Optional Accessories*.) The phase adjusters have male and female SMA connectors to simplify connections to your measurement system.

You must add a phase adjuster on each cable to balance the delay and insertion loss introduced by the phase adjuster. You only adjust (add delay to) the phase adjuster on the cable with the shorter delay.

The adjustment range of the phase adjusters on the *Optional Accessories* list is 25 ps, so if you use cable pairs other than those supplied with the probe, the initial delay mismatch should be less than 25 ps.

1. Connect the phase adjusters to the cables.
2. On the cable with the longer delay, loosen the phase adjuster locking nuts, set the phase adjuster to minimum delay (shortest length), and secure the locking nuts. (See Figure 12.)

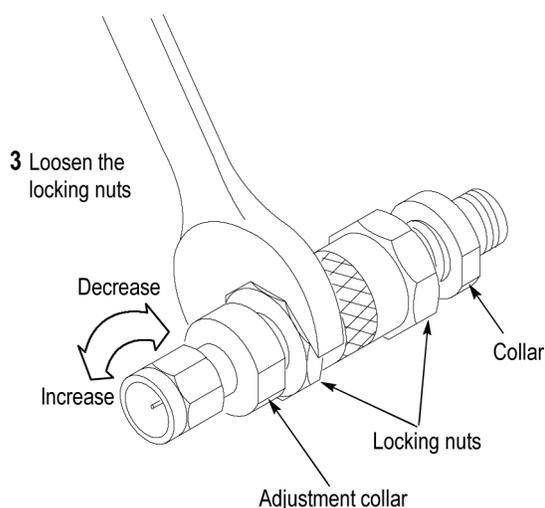

- 4 Turn adjustment collar while observing oscilloscope display

Figure 12: Using the phase adjuster

3. Loosen the locking nuts on the adjuster that is connected to the other cable (with the shorter delay).
4. While observing the oscilloscope display, turn the collar on the phase adjuster counterclockwise to increase the delay.
5. When the displayed skew on screen is less than 1 ps, tighten the locking nuts.
6. Confirm that the skew is acceptable after you tighten the locking nuts, as the adjustment may change slightly during tightening.
7. Disconnect the cables from the sampling head, and connect them to the P7313SMA probe head.

Deskewing Probes

You can measure the skew between two P7313SMA probes by using a Tektronix 80E10 Sampling Head configured for a TDR output. Because the skew of the P7313SMA probe inputs is less than 1 ps, two P7313SMA probes can be deskewed using single-ended drive signals from a dual-channel TDR source. The TDR output provides a pair of time-aligned pulses that you can use to compare probe response times, and if necessary, adjust them to match (deskew).


A setup is shown for checking and deskewing two probes. (See Figure 13.) Deskewing aligns the time delay of the signal path through the oscilloscope channel and probe connected to that channel, to the time delay of other channel/probe pairs of the oscilloscope.

If you need to deskew more than two probes, keep one deskewed probe connected to the sampling head as a reference (after deskewing two probes), and deskew additional probes to that probe. In this procedure, Channel 1 is used as the reference channel.

1. Set up the equipment and let it warm up for 20 minutes, but don't make any connections to the TDR outputs yet.
2. Do a system compensation for the TDR module, and then verify the skew of the two outputs with the TDR outputs open, using a common-mode TDR drive.

Skew between the two outputs can be compensated with the deskew control. Refer to your sampling head or oscilloscope manual for instructions.

3. Attach the probes to the TDR outputs. (See Figure 13.)

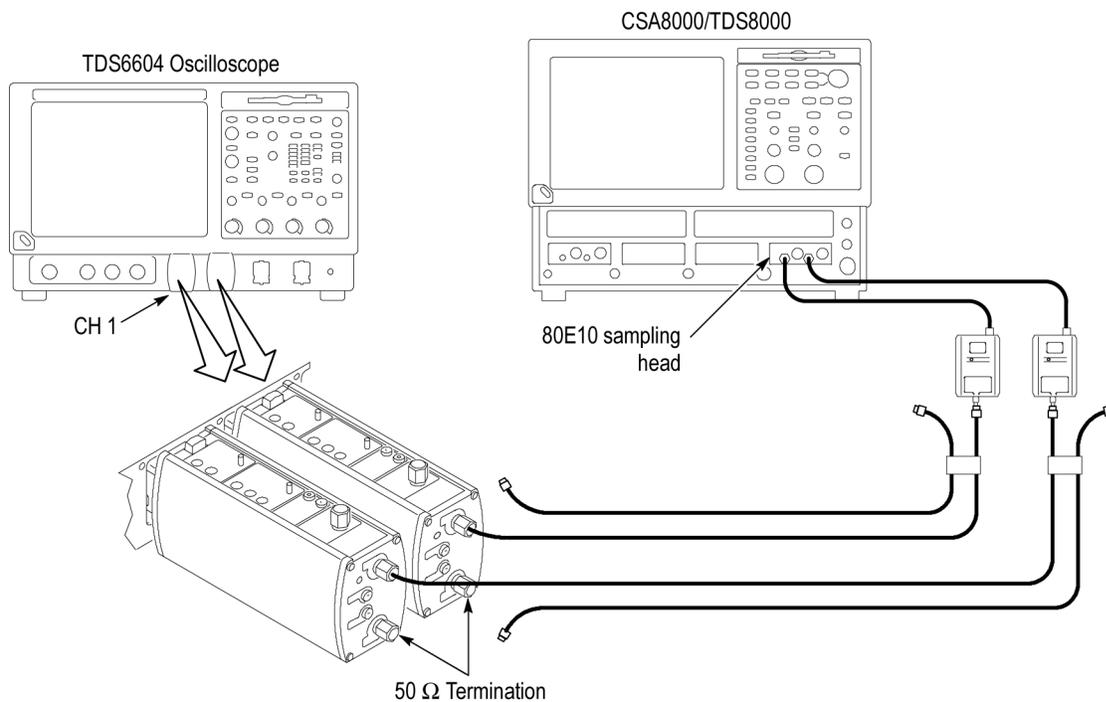

Note: * Use the cables that you will use to connect to your circuit

1968-001

Figure 13: Deskewing two P7313SMA probes

4. Display the channel(s) that you want to deskew.
5. Push the **AUTOSET** button on the instrument front panel.

6. Turn averaging on to stabilize the display.
7. Adjust vertical **SCALE**, and **POSITION** (with active probes, adjusting **offset** may be required) for each channel so that the signals overlap and are centered on-screen.
8. Adjust horizontal **POSITION** so that a triggered rising edge is at center screen.
9. Adjust horizontal **SCALE** so that the differences in the channel delays are clearly visible.
10. Adjust horizontal **POSITION** again so that the rising edge of the Channel 1 signal is exactly at center screen. Now, if you want to, you can use the measurement cursors to display the channel-channel skew, and enter this value in step 14.
11. Touch the **VERT** button or use the **Vertical** menu to display the vertical control window.
12. Touch the Probe **Deskew** button to display the channel-deskew control window.
13. In the **Channel** box, select the channel that you want to deskew to Channel 1.

NOTE. *If possible, do the next step at a signal amplitude within the same attenuator range (vertical scale) as your planned signal measurements. Any change to the vertical scale after deskew is complete may introduce a new attenuation level (you can generally hear attenuator settings change) and, therefore, a slightly different signal path. This different path may cause up to a 200 ps variation in timing accuracy between channels.*

14. Adjust the deskew time for the signal that you want to deskew so that the signal aligns with the Channel 1 signal. You can do this several ways:
 - Click the **Deskew** field and input the time value you measured with the cursors in step 10.
 - Use the front-panel controls to position the signal.
 - Use the on-screen controls to position the signal.
15. Repeat steps 3 through 14 for each additional channel that you want to deskew.

Reference

This section contains reference information about communication standards and related differential measurements.

Serial Bus Standards

Some popular high-speed data communication standards that can be measured with the P7313SMA differential probe are listed below. (See Table 3.)

Table 3: Serial bus standards with dynamic range requirements

| Standard | Data Rate | Vdm_max | Vdm_min | Vcm_max | Vcm_min |
|------------------|------------|--------------|---------|------------|------------|
| HDMI | 1.65 Gb/s | 800 mV | 150 mV | 3.3 V | 2.8 V |
| InfiniBand TX | 2.5 Gb/s | 1.6 V | 1.0 V | 1.0 V | 0.5 V |
| InfiniBand RX | 2.5 Gb/s | 1.6 V | 0.175 V | 1.0 V | 0.5 V |
| PCI Express TX | 2.5 Gb/s | 1.2 V | 0.8 V | AC | AC |
| PCI Express RX | 2.5 Gb/s | 1.2 V | 0.175 V | AC | AC |
| Serial ATA TX | 1.5 Gb/s | 0.6 V | 0.4 V | 0.3 V | 0.2 V |
| Serial ATA RX | 1.5 Gb/s | 0.6 V | 0.325 V | 0.3 V | 0.2 V |
| XAUI TX | 3.125 Gb/s | | 0.4 V | | |
| XAUI RX | 3.125 Gb/s | | 0.1 V | | |
| OIF-SxI-5 TX | 3.125 Gb/s | 1.0 V | 0.5 V | 1.23 V | 0.72 V |
| OIF-SxI-5 RX | 3.125 Gb/s | 1.0 V | 0.175 V | 1.30 V | 1.10 V |
| LV PECL (stdECL) | >12GHz | 1.66 V (typ) | 1.48 V | 1.3 V (vt) | 0.5 V (vt) |
| LV PECL (RSECL) | >12GHz | 1.05 V | 0.70 V | 1.3 V (vt) | 0.5 V (vt) |

InfiniBand

A number of high-speed serial data communication standards have been introduced to address the need for next generation I/O connectivity. One of these interface standards, InfiniBand, is briefly discussed here. (See Figure 14.)

An InfiniBand communication lane includes two independent differential signaling paths, one for transmit and one for receive, both operating at a 2.5 Gb/s rate. As shown in the example below, the differential output parameter is specified as a peak-to-peak voltage difference, and thus the signal swing on each pin of the driver is half that value.

The V_{diff} signal shown in (b) is measured with a differential probe connected between the two signals in (a). The V_{diff} signal represents the result of the receiver processing the two complementary input signals from the driver shown in (a), and cannot be measured directly as a single-ended signal.

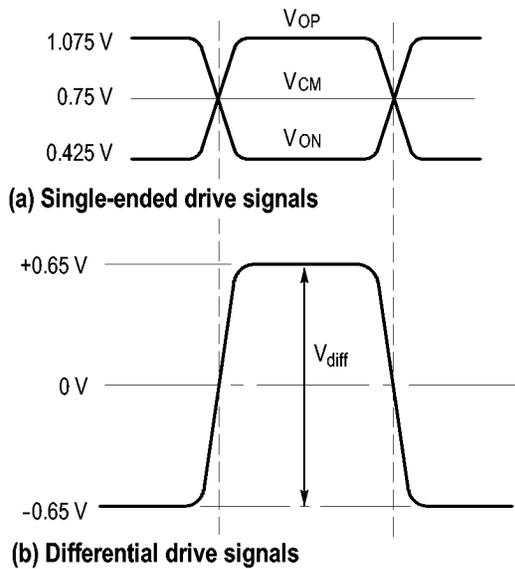


Figure 14: InfiniBand signals

Specifications

The specifications in the following tables apply to a P7313SMA probe installed on a TDS6804 oscilloscope. The probe must have a warm-up period of at least 20 minutes and be in an environment that does not exceed the limits described. (See Table 4.) Specifications for the P7313SMA differential probe fall into three categories: warranted, typical, and nominal characteristics.

Warranted Characteristics

Warranted characteristics describe guaranteed performance within tolerance limits or certain type-tested requirements. (See Table 4.) Warranted characteristics that have checks in the *Performance Verification* section are marked with the ✓ symbol.

Table 4: Warranted electrical characteristics

| Characteristic | Description |
|--|---|
| ✓ Differential rise time, 10-90% (probe only) (Main output) | ≤40 ps, +20 °C to +30 °C (+68 °F to +86 °F), 100 mV differential step in 2.5X attenuation 500 mV differential step in 12.5X attenuation |
| Differential signal range | 0.800 V _{p-p} (2.5X attenuation) 3.6 V _{p-p} (12.5X attenuation) |
| ✓ DC gain (Main output) | 0.40 ±2.0% (corresponds to 2.5 X attenuation) 0.08 ±2.0% (corresponds to 12.5 X attenuation) |
| Termination voltage range | +3.6 V /-2.5 V |
| ✓ Termination voltage accuracy | |
| (EXT mode) | ±(0.2% x V _T + 2 mV) over a +3.6 V/-2.5 volt V _T range |
| (INT mode) | ±(0.3% x V _T + 2 mV) over a +3.6 V/-2.5 volt V _T range |
| (AUTO mode) | ±(2.5% x V _{CM} + 20 mV) over a +3.6 V/-2.5 volt V _{CM} range |
| Linearity | ±1% or less of dynamic range |
| ✓ Output offset voltage (Main output) V _{CM} = 0 V, V _{DM} = 0 V, V _T = 0 V | ±2.5 mV +20 °C to +30 °C (+68 °F to +86 °F) |
| ✓ Differential-mode input resistance | 100 Ω ±2% |
| Maximum nondestructive input voltage V _T = 0 V, applied <5 minutes | ±5 V (DC + peak AC) on either SMA input |
| Maximum nondestructive external termination input voltage | ±15 VDC |
| Temperature | Operating: 0 to +40 °C (+32 to +104 °F) Nonoperating: -55 to +75 °C (-131 to +167 °F) |
| Humidity | Operating: 0-90% RH, tested at +30 to +40 °C (+68 to +104 °F) Nonoperating: 0-90% RH, tested at +30 to +60 °C (+68 to +140 °F) |

Typical Characteristics

Typical characteristics describe typical but not guaranteed performance. (See Table 5.)

Table 5: Typical electrical characteristics

| Characteristic | Description |
|---|---|
| Differential bandwidth (probe only) | |
| Main output | DC to 13 GHz (-3 dB) |
| Aux output | DC to 13 GHz (-6 dB) |
| Differential rise time, 20-80% (probe only, Main and Aux output) | ≤25 ps, +20 °C to +30 °C (+68 °F to +86 °F), 100 mV differential step in 2.5X attenuation 500 mV differential step in 12.5X attenuation |
| Single-ended rise time, 10-90%, (probe only, Main and Aux output) | ≤40 ps, +20 °C to +30 °C (+68 °F to +86 °F), 250 mV step |
| Differential signal input skew | <1 ps (with matched SMA cable pair) |
| Differential input return loss | >35 dB @500 MHz (VSWR <1.06:1) >20 dB @6.5 GHz (VSWR <1.22:1) >15 dB @10 GHz (VSWR <1.43:1) >12 dB @13 GHz (VSWR <1.67:1) |
| Termination voltage driver current | ±(82.5 mA ±8 mA) overload |
| Common-mode DC input signal range | +3.6 V/-2.5 V |
| Common-mode input return loss | >35 dB @500 MHz (VSWR <1.06:1) >20 dB @6.5 GHz (VSWR <1.22:1) >15 dB @10 GHz (VSWR <1.43:1) >12 dB @13 GHz (VSWR <1.67:1) |
| Common-mode rejection ratio (Main output) (See Figure 15 on page 27.) | >45 dB @1 GHz >40 dB @2.5 GHz >30 dB @5 GHz >20 dB @10 GHz >15 dB @13 GHz |
| Common-mode rejection ratio (Aux output) | >45 dB @1 GHz >40 dB @2.5 GHz >30 dB @5 GHz >20 dB @10 GHz >15 dB @13 GHz |
| Delay time (includes standard cables) | 5.15 ns ±100 ps, relative to a TCA-SMA adapter |
| Noise, referred to input | 13 nV/√Hz (2.5 X attenuation) 40 nV/√Hz (12.5 X attenuation) |
| DC gain (Aux output) | 0.40 ±2.5% (corresponds to 2.5 X attenuation) 0.08 ±2.5% (corresponds to 12.5 X attenuation) |
| Output offset voltage (Aux output) | ±15 mV, +20 °C to +30 °C (+68 °F to +86 °F) |
| Output offset voltage (Main output) $V_{CM} = 0\text{ V}$, $V_T = \pm 2.0\text{ V}$ | <±5 mV, +20 °C to +30 °C (+68 °F to +86 °F) |
| $V_{CM} = \pm 2.5\text{ V}$, $V_T = 0\text{ V}$ | <±5 mV, +20 °C to +30 °C (+68 °F to +86 °F) |

Table 5: Typical electrical characteristics (cont.)

| Characteristic | Description |
|---|--|
| DC offset drift | -50 mV/°C or less at output of probe (results in -0.125 mV/°C or less (2.5 X), or -0.625 mV/°C or less (12.5 X) displayed on screen) |
| DC voltage measurement accuracy (referred to input) | ±(2% of input + 8.00 mV + 8.00 mV) (2.5 X) ±(2% of input + 36.00 mV + 36.0 mV) (12.5 X) gain error = ±2% of input voltage output zero offset (referred to input) = ±8.00 mV (2.5 X) ±36.00 mV (12.5 X) linearity error = ±1.0% of: 800 mV dynamic range = 8.00 mV (2.5 X) 3.6 V dynamic range = 36.0 mV (12.5 X) |

Typical differential CMRR plot for the probe. (See Figure 15.)

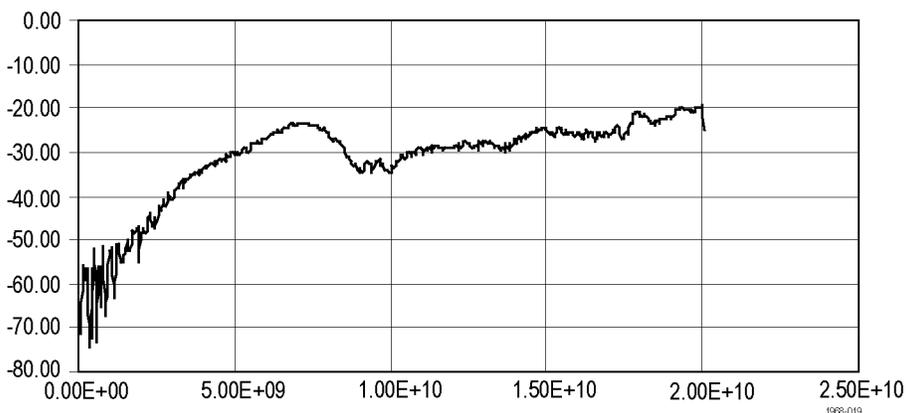


Figure 15: Typical CMRR plot

Typical differential input return loss plot for the probe. (See Figure 16.)

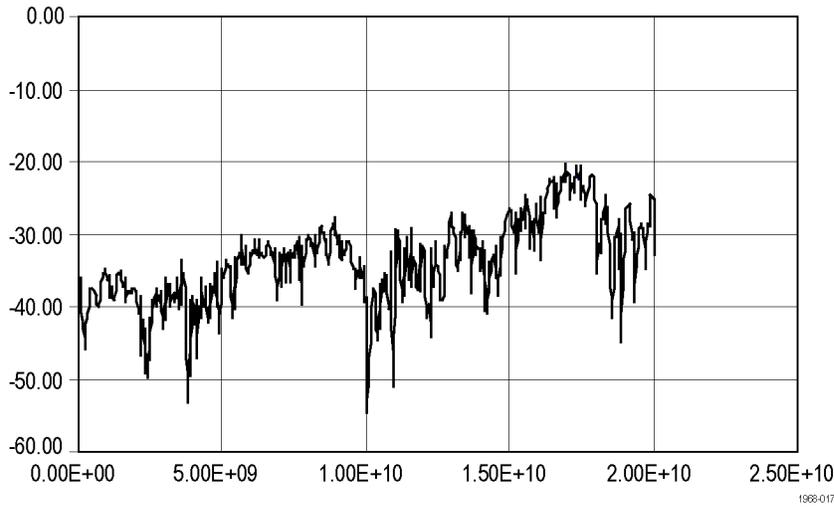


Figure 16: Typical differential input return loss

Typical differential-mode bandwidth plot for the probe. (See Figure 17.)

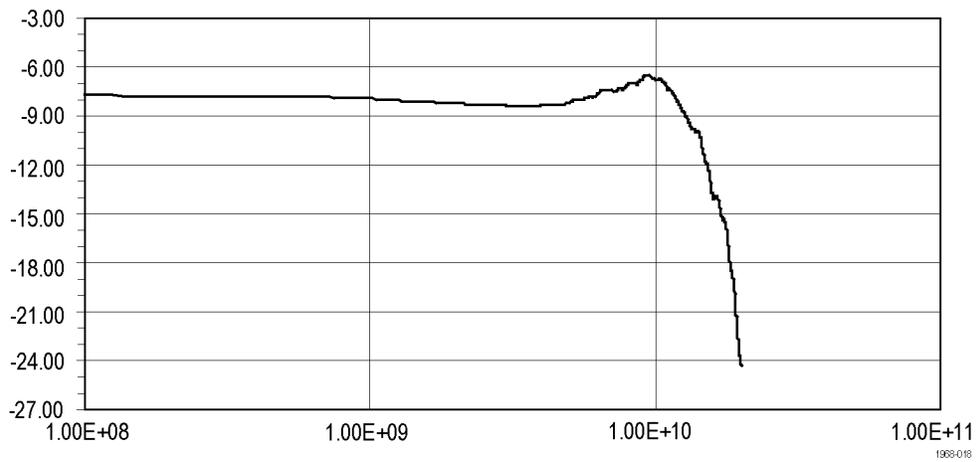


Figure 17: Typical differential-mode bandwidth

Typical eye pattern as measured with the probe. (See Figure 18.)

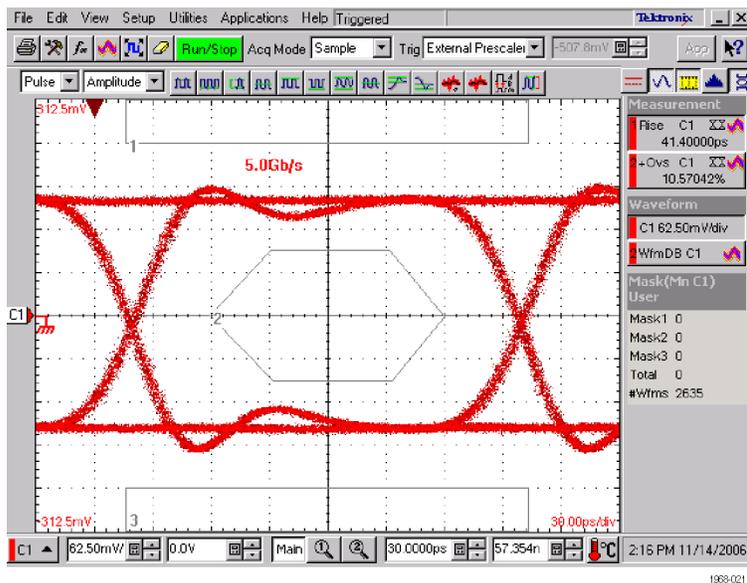


Figure 18: Typical eye pattern

Typical step response as measured with the probe. (See Figure 19.)

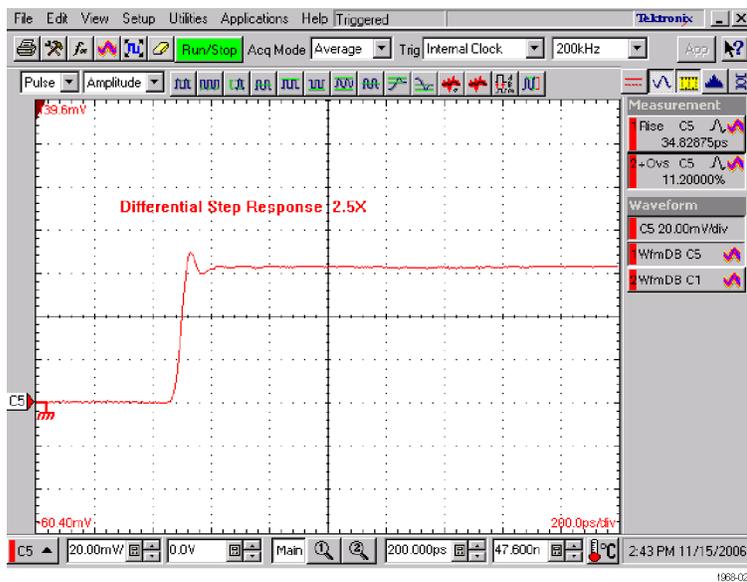


Figure 19: Typical differential step response

Nominal Characteristics

Nominal characteristics describe guaranteed traits, but the traits do not have tolerance limits. (See Table 6.)

Table 6: Nominal electrical characteristics

| | |
|---|--|
| Signal input configuration | Differential (two SMA inputs, + and -) |
| Input coupling | DC |
| Attenuation | 2.5 X and 12.5 X ¹ |
| Common-mode input resistance | 50 Ω \pm 1% (internally per side) |
| Termination voltage input configuration | DC (two 0.080 in jacks, + and -) |
| Termination voltage buffer input resistance | 100 K Ω |
| Termination voltage output monitor | DC (two 0.040 in jacks, + and -) |
| Termination voltage output monitor resistance | 1 K Ω |
| Output coupling and termination | DC, terminate output into 50 Ω |
| Auxiliary signal output | SMA output |

¹ All TekConnect host instruments recognize this gain setting and adjust the Volts/Div setting to correspond to a normal 1-2-5 sequence of gains.

Mechanical Characteristics

The mechanical characteristics of the probe are listed below. (See Table 7.) The mechanical dimensions are shown. (See Figure 20.)

Table 7: Typical mechanical characteristics

| | |
|---|---|
| Dimensions | 48.0 mm × 31.8 mm × 129.5 mm (1.9 in × 1.3 in × 5.1 in) |
| Unit weight | 230 g (0.51 lb) |
| Shipping weight (includes shipping materials) | 1.38 kg (3.1 lb) |
| Standard cable assembly length | 0.96 m (38 in) |

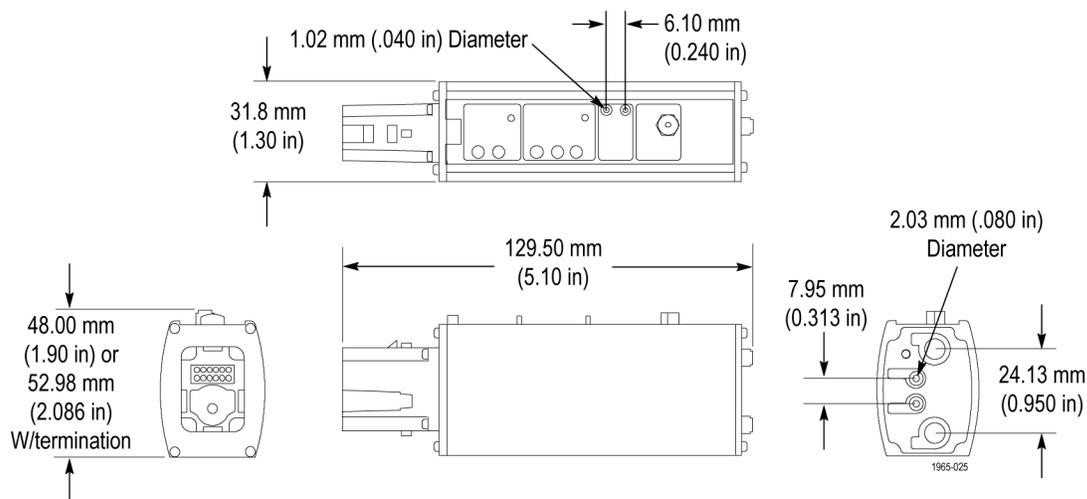


Figure 20: Probe dimensions

Performance Verification

Use the following procedures to verify specifications of the probe. The recommended calibration interval is one year.

These procedures test the following specifications:

- Differential mode input resistance
- Termination voltage accuracy
- Output offset zero
- DC gain accuracy
- Differential mode rise time

Equipment Required

A list of the equipment required to verify the performance of your probe is shown. (See Table 8.)

Table 8: Equipment required for performance verification

| Item description | Performance requirement | Recommended example ¹ |
|---|---|--|
| Oscilloscope | TekConnect interface | Tektronix TDS6804 or TDS7704 |
| Sampling Oscilloscope | Windows 2000 OS, with oscilloscope FW \geq V2.5 (for compatibility with Tektronix 80E08/10 modules) | Tektronix TDS8000 |
| Sampling Module | 30 GHz bandwidth | Tektronix 80E08 |
| Sampling Module | 20 GHz bandwidth | Tektronix 80E04 |
| TekConnect Probe Interface Module with semi-rigid cable | Firmware version V2.2 or above | Tektronix 80A03, with 174-4857-xx cable |
| DMM (2), with leads | 0.1 mV and 0.01 Ω resolution | Fluke 187 or equivalent |
| Dual Power Supply | 5.0 VDC at 200 mA | B+K Precision 1760A or equivalent |
| Feedthrough Termination | BNC, 50 Ω \pm 0.05 Ω | 011-0129-00 |
| Attenuators (2) | SMA, 50 Ω , 5X attenuation | 015-1002-01 |
| Coaxial cable | Male-to-Male SMA | 012-0649-00 |
| Coaxial cable | Dual, matched-delay Male-to-Male SMA | 174-4944-00 ² |
| Coaxial cable | Male-to-Male BNC, 50 Ω | 012-0057-01 |
| Test leads (2) | Banana plug ends, red | 012-0031-00 |
| Test leads (2) | Banana plug ends, black | 012-0039-00 |
| Test leads | 0.080 in pin-to-Banana plug ends, one each color | 012-1674-00 (red) ² 012-1675-00 (black) ² |
| Adapter | (See Figure 21 on page 33.) | Tektronix TCA-SMA |
| Adapters (3) | SMA 50 Ω termination | 015-1022-00 ² |
| Adapter | SMA Male-to-SMA Male | 015-1011-00 ² |
| Adapters (2) | 0.040 in-to-0.080 in pin jack | 012-1676-xx ² |

Table 8: Equipment required for performance verification (cont.)

| Item description | Performance requirement | Recommended example ¹ |
|-------------------|---------------------------|----------------------------------|
| Adapter | SMA Male-to-BNC Female | 015-1018-00 |
| Adapters (2) | BNC Male-to-SMA Female | 015-0572-00 ³ |
| Adapters (3) | BNC Female-to-Dual Banana | 103-0090-00 |
| Adapter | BNC T | 103-0030-00 |
| Adapter | BNC Female-to-BNC Female | 103-0028-00 |
| SMA torque wrench | 5/16-in, 7 in-lb. | |

¹ Nine-digit part numbers (xxx-xxxx-xx) are Tektronix part numbers.

² Standard accessory included with the probe.

³ One adapter is included with the probe.

Special Adapters Required

Some of the adapters listed in the previous table are available only from Tektronix. These adapters are described on the following pages.

TekConnect-to-SMA Adapter

The TekConnect-to-SMA Adapter, Tektronix part number TCA-SMA, allows signals from an SMA cable or probe to be connected to a TekConnect input. (See Figure 21.) Connect and disconnect the adapter the same way as you do the probe.

This adapter is an oscilloscope accessory that may be used for measurement applications, as well as these performance verification procedures.




Figure 21: TekConnect-to-SMA Adapter

Equipment Setup

The following tests use two oscilloscopes; use this procedure to set up and warm the equipment to test the probe. Wear the antistatic wriststrap when performing these procedures.

1. Connect the 80A03 TekConnect probe interface to channels 3 and 4 of the TDS8000 oscilloscope. (See Figure 22.)
2. Connect the 80E04 module to the 80A03 TekConnect probe interface.
3. Connect the 80E08 module to channels 7 and 8 of the TDS8000 oscilloscope.
4. Connect a 50 Ω termination to the Aux Output connector on the probe, and connect the probe to one of the 80A03 channels.
5. Turn on both oscilloscopes and allow 20 minutes for the equipment to warm up.
6. Photocopy the test record to record the performance test results. (See Table 9 on page 47.)

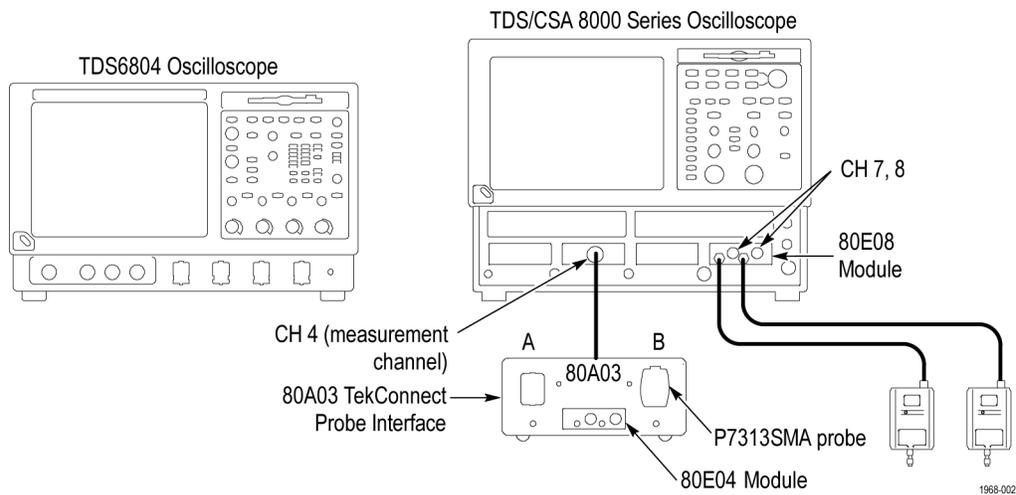


Figure 22: Preliminary test setup

Input Resistance

This test checks the differential mode input resistance (the resistance between each SMA input). The test is performed with the probe disconnected from the oscilloscope.

1. Disconnect the probe from the oscilloscope.
2. Zero the DMM with its measurement leads connected together on the lowest scale that can measure 100 Ω .
3. Remove the SMA terminations from the two probe inputs and gently probe the center contacts of the input connectors. Be careful not to touch the outer edge (ground) of the connector. (See Figure 23.)
4. Measure the resistance and write down the value.
5. Reverse the DMM connections and repeat the measurement. Write down the value.
6. Add the two measurements from steps 4 and 5, and divide the total by two. Record the result in the test record.
7. Connect the probe to the oscilloscope channel that you will use in the next test so that the probe warms up to operating temperature.

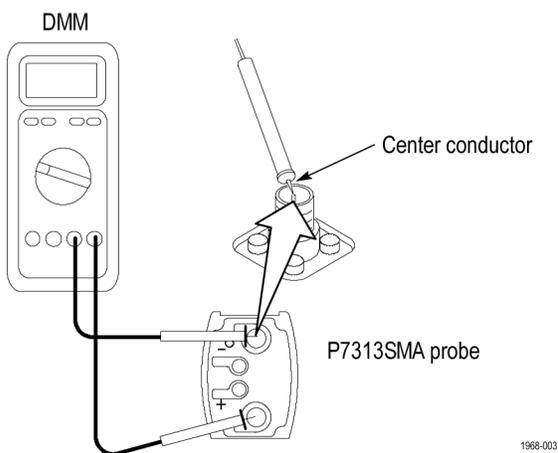


Figure 23: Checking differential mode input resistance

Termination Voltage Accuracy

These tests compare the termination control voltage that you apply (using the adjustment control for that termination voltage mode), to the termination voltage output at the Vterm monitor jacks.

NOTE. The Auto mode LED will flash when the probe inputs are open-circuit, or below a 50 mV threshold. If the LED continues to flash after you connect the inputs, cycle the mode SELECT button.

External (Ext) Mode

The Ext mode test setup is shown. (See Figure 24.)

1. Plug the probe directly into an oscilloscope channel and set the Vterm Source Select to EXT on the probe.

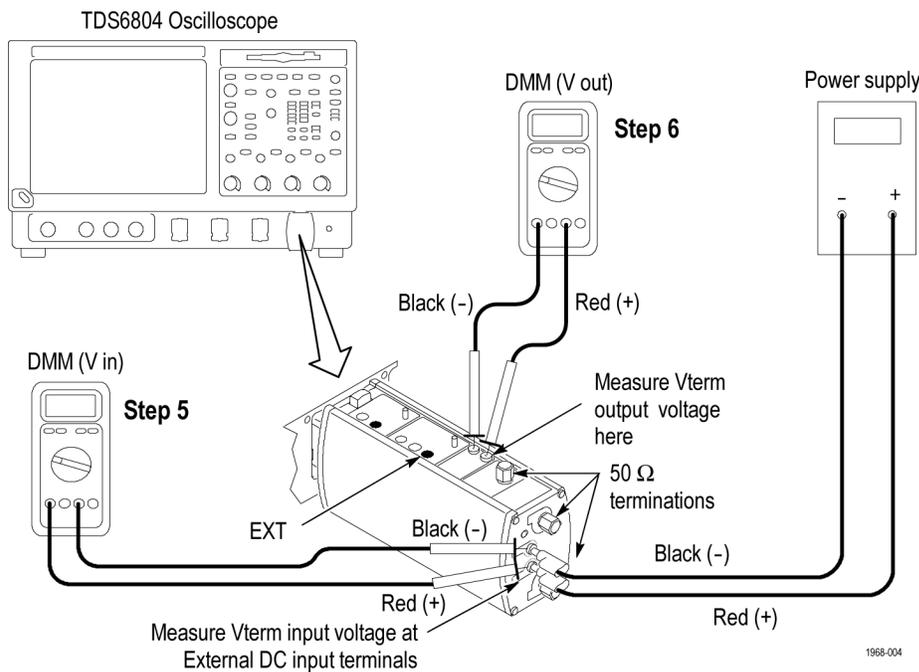


Figure 24: Termination Voltage Accuracy, Ext mode setup

2. Connect the 50 Ω terminations on the three probe SMA connectors. This sets the common mode input voltage to 0.0 V.
3. The probe attenuation can be set to either 2.5X or 12.5X.
4. Using the 0.080 in pin-to-Banana plug cables, connect the power supply to the external DC input jacks on the front of the probe.
5. Set the power supply as close as practical to 0.000 volts, and use the DMM to measure this input voltage at the terminals on the front of the probe. Record this voltage as V_{in} on the test record.

6. Use the second DMM to measure the output voltage at the termination voltage monitor jacks on the top of the probe. Record this voltage as V_{out} on the test record, and verify that the V_{out} voltage is within the specified limits in the min/max columns. For example, within ± 2 mV of the actual V_{in} voltage that you measured in the previous step.
7. Repeat steps 5 and 6 for the +2.500 volt and -2.500 volt input values listed in the test record.

Internal (Int) Mode

If your oscilloscope supports internal mode, use this test to check the accuracy of the internally-generated termination voltages. In Int mode, you use a graphical user interface in the oscilloscope to set the test values to the 0.000, +2.500 and -2.500 volt levels, instead of using external power supplies. You do not need to measure these values in Int mode, as they are digitally set.

See your oscilloscope manual for details on using the interface.

1. Disconnect the power supply from the probe.
2. Set the V_{term} Source Select to INT on the probe.
3. Use the graphical user interface in the oscilloscope to set the termination voltage to 0.000 V.
4. Use the DMM to verify that the termination voltage output at the V_{term} monitor jacks on the top of the probe is within the limits on the test record. Record this value as V_{out} on the test record.
5. Repeat steps 3 and 4 for the +2.500 volt and -2.500 volt input values listed in the test record.

Auto Mode

In Auto mode, the probe measures the input signal DC common mode voltage and automatically sets the termination voltage to equal that voltage. In this test, the two signal inputs are connected together and driven by an external power supply to set the common mode voltage to the 0.0, +2.500 and -2.500 volt test values.

1. Connect the test setup as shown. (See Figure 25.)

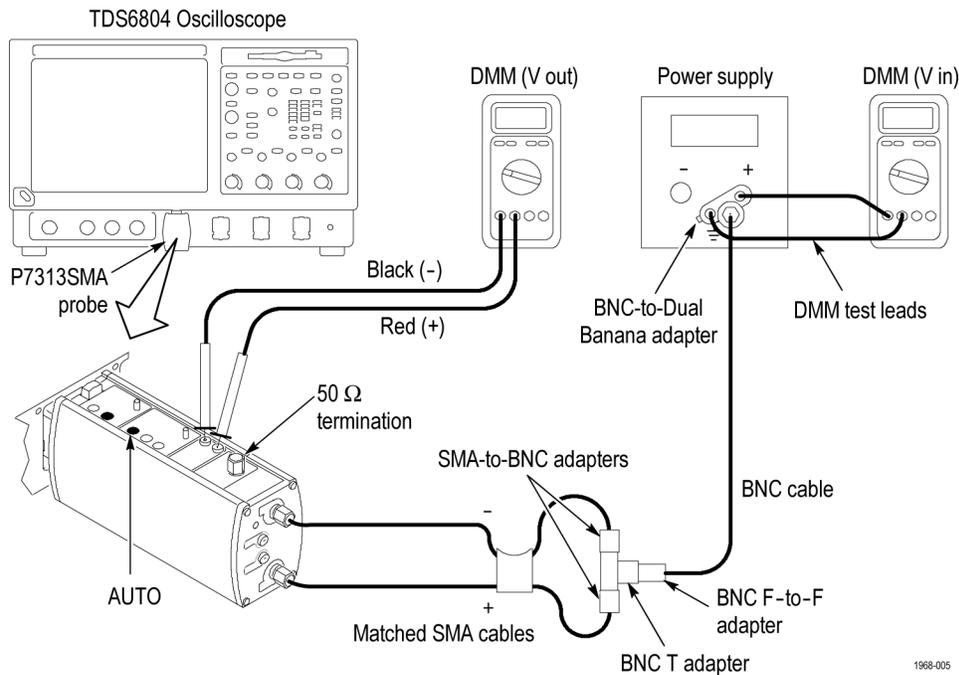


Figure 25: Termination Voltage Accuracy, Auto mode setup

2. Set the Vterm Source Select to Auto on the probe.
3. Set the power supply as close as practical to 0.000 volts, and use the DMM to measure this input voltage at the terminals on the power supply. Record this voltage as V_{in} on the test record.
4. Use the second DMM to measure the output voltage at the termination voltage monitor jacks on the top of the probe. Record this voltage as V_{out} on the test record, and verify that the V_{out} voltage is within the specified limits in the min/max columns.
5. Repeat steps 3 and 4 for the +2.500 volt and -2.500 volt input values listed in the test record.

Output Offset Zero

By terminating the two probe SMA inputs with $50\ \Omega$, this procedure tests the zero output voltage of the probe. The probe output is measured at the SMA connector on the front of the 80A03 interface.

1. Connect the equipment as shown. (See Figure 26.)
2. Connect two $50\ \Omega$ terminations to the two probe SMA inputs on the probe, and plug the probe into the 80A03 module.
3. Connect the cable from the DMM to the SMA connector that is located below the 80A03 channel that you plugged the probe into.

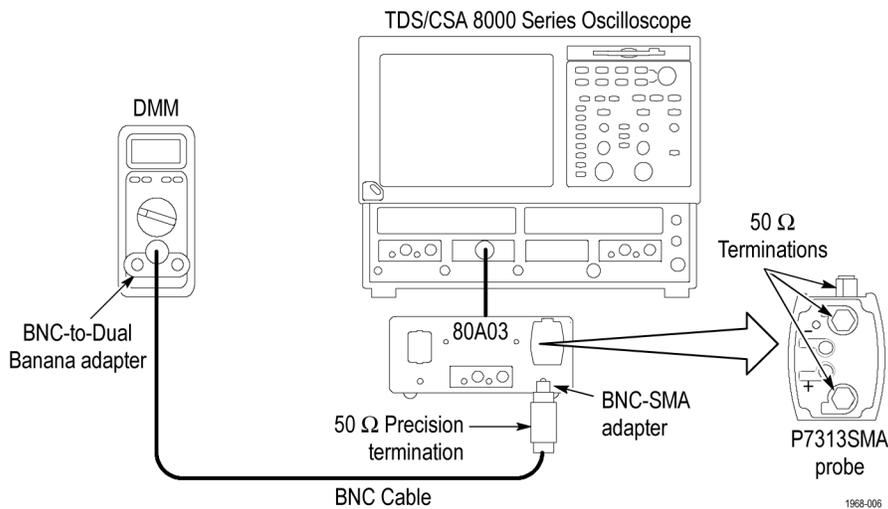


Figure 26: Setup for the output offset zero test

4. Set the V_{term} source to Ext on the probe. Leave the external termination control voltage inputs open. This sets the termination voltage to zero.
5. Set the multimeter to read DC volts.
6. Verify that the output voltage is $0\ V, \pm 2.5\ mV$ for both the 2.5X and 12.5X attenuation settings.
7. Record the results on the test record.

DC Gain Accuracy

This test checks the DC gain accuracy of the probe at the two attenuation settings, 2.5X and 12.5X.

Gain Check at 2.5X Attenuation

1. Set the attenuation on the probe to 2.5X, and the termination select to Auto.
2. Connect the probe to the power supplies as shown. (See Figure 27.) Make sure the ground tabs on the BNC-to-dual banana plug adapters are connected to the ground connections on the power supplies. Monitor the source voltage with one of the DMMs.

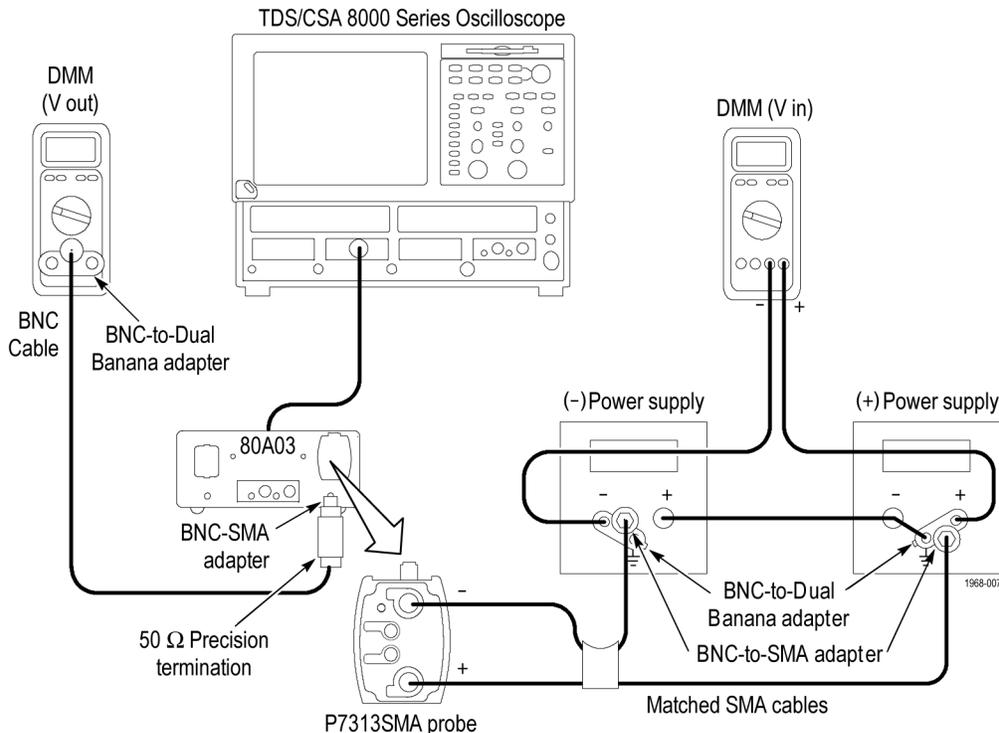


Figure 27: DC Gain Accuracy setup

3. Set the voltage on each power supply to approximately +0.160 V (+0.32 V differential total). This represents 80% of the probe dynamic range in this attenuation setting. Record this source voltage as V_{in1} .
4. Record the output voltage (on the second DMM) as V_{out1} .
5. Disconnect the BNC-to-dual banana plug adapters from the power supplies. Leave the DMM leads connected to the adapters.
6. Connect the BNC-to-dual banana plug adapters into the opposite power supplies to reverse the voltage polarity to the probe inputs. (See Figure 28 on page 41.)
7. Record the actual source voltage (now a negative value), as V_{in2} .

Rise Time

This procedure verifies that the probe meets the differential rise time specification. Two rise times are measured; the test system alone, and the test system with the probe included. The probe rise time is calculated using the two measurements.

Note: This test uses the TDR function of the 80E08 or 80E10 sampling head as a fast rise time signal source. A second 80E0X sampling head is used to take the measurements, using an 80A03 TekConnect probe interface. Although the following procedure assigns the TDR and measurement functions to specific oscilloscope channels, any valid channel combination can be used. However, the TDR rise times required of the sampling heads in this test are only available on 80E08 and 80E10 sampling heads.

This test checks both of the probe attenuation settings, but due to the differential TDR output amplitude and common mode voltage, inline 5X attenuators must be used when checking the 2.5X attenuation setting on the probe.

Rise Time Check at 12.5X Attenuation

1. Connect the test equipment as shown. (See Figure 29.)



CAUTION. To prevent mechanical strain on the connectors, use care when working with SMA connectors: support equipment and use a torque wrench to tighten connections to 7 in-lbs.

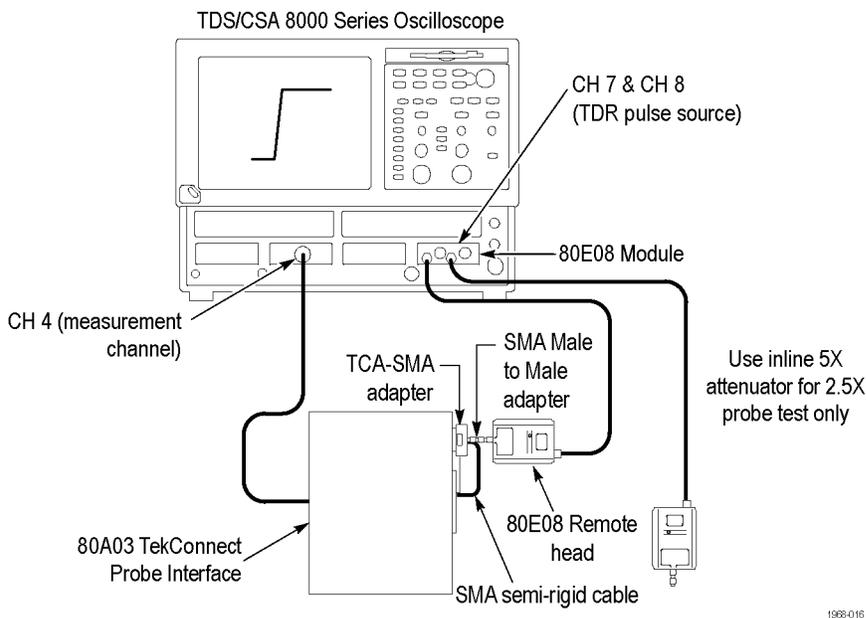


Figure 29: Test system rise time setup

NOTE. The firmware of the 80A03 TekConnect Probe Interface used to power the probe must be version V2.2 or above.

2. Turn on Channel 4 and set the vertical scale to 50 mV/div.
3. Set the Channel 7/8 sampling head to TDR mode: Press the SETUP DIALOGS button and select the TDR tab. (See Figure 30.)

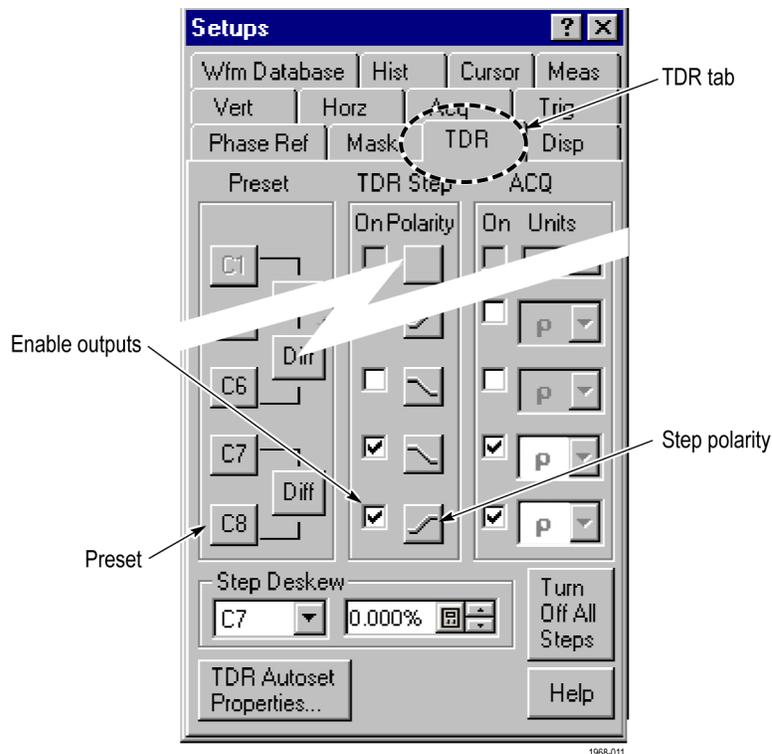


Figure 30: Setting the TDR parameters

4. Set the Channel 7 (**C7**) **Polarity** to negative (falling).
5. Set the Channel 8 (**C8**) **Polarity** to positive (rising).
6. Set the **Preset** of Channel 7 and 8 on.

TDR Preset sets Internal Clock in the Trigger menu, turns on the TDR Step in the TDR Setups menu, turns on the channel and selects the acquisition Units in the TDR Setups menu, and sets the horizontal scale, position, and reference. The sampling module will turn on a red light next to the SELECT channel button, indicating that TDR is activated for that channel.

Deskew Channel 7 and 8 by doing the following:

7. Check that Ch 7 is set to negative slope and Ch 8 is set to positive slope.
8. Verify/clear all deskew values for Ch 7 and Ch 8 in both the TDR menu and the vertical menu.
9. Turn off the display for Ch 7 and Ch 8 so that only Ch 4 is shown on screen.
10. Set the horizontal scale to 10 ps/div, and the vertical scale to 50 mV/div.
11. Adjust Ch 4 to position the step at 0 V, and then enter -125 mV offset to position the step as shown. (See Figure 31.) Save this waveform to a reference.

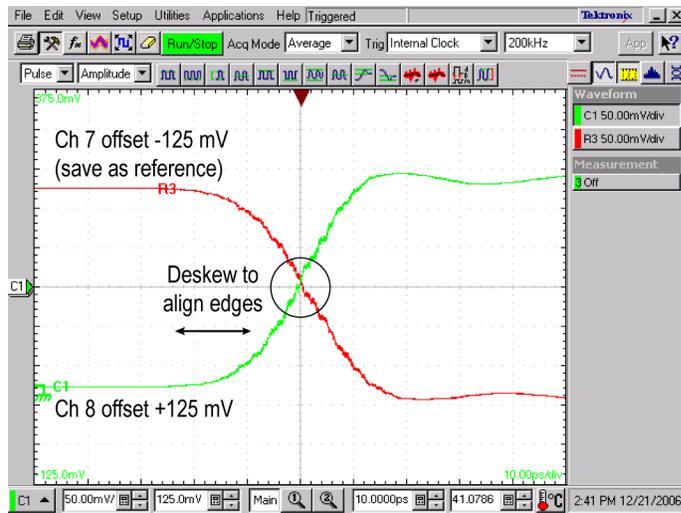


Figure 31: Deskew the TDR steps

12. Remove Ch 7 from the Ch 4 input and connect Ch 8 to the Ch 4 input.
13. Press the Ch 4 button to display Channel 4.
14. Enter 125 mV offset to position the step as shown. (See Figure 31.)
15. From the TDR menu, adjust the deskew on Ch 8 to align the edges with the reference value from step 11.
16. Use the oscilloscope measurement capability to display rise time. Increase the stability of the pulse edge measurement by using averaging, if available. Rise time is measured from the 10% and 90% amplitude points on the waveform. Record the rise time as t_s .

The following steps instruct you to assemble the test setup that includes the probe. (See Figure 32.) The system and probe rise time (t_{s+p}) that you measure in step 24 is used to calculate the probe rise time (t_p) in step 25.

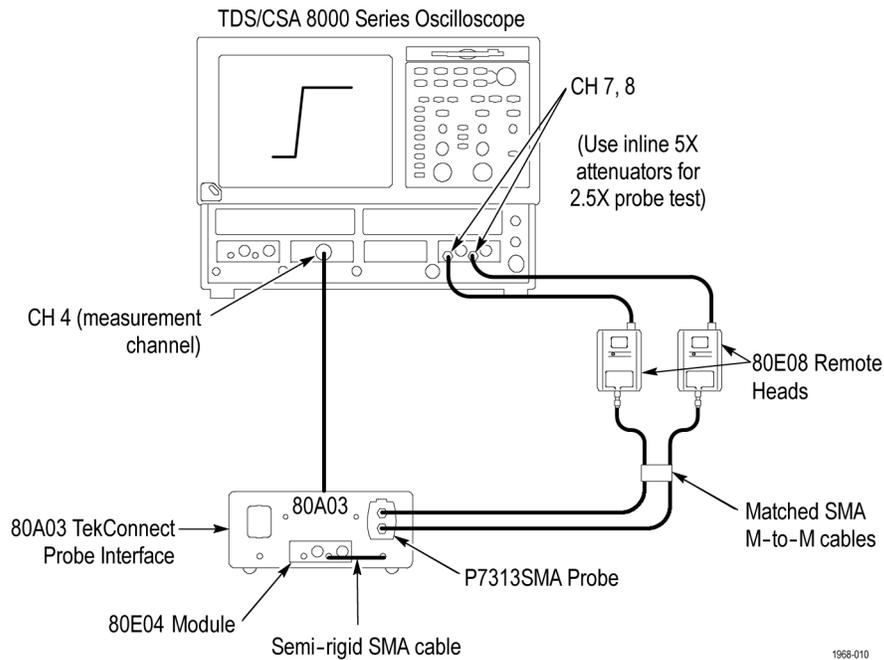


Figure 32: Test system rise time setup with probe

17. Remove the TekConnect-to-SMA adapter from the test setup.
18. Connect the probe to the 80A03 TekConnect probe interface.
19. Connect the matched SMA cables to the probe SMA inputs and the 80E08 sampling head (Channels 7 and 8).
20. Set the attenuation on the probe to 12.5X.

The test setup should now be connected as shown. (See Figure 32.)

21. Expand the horizontal scale to help locate the step edge, and then adjust horizontal range to 50 ps/div while maintaining the edge view. For a more stable measurement display, turn averaging on.
22. Adjust the vertical scale to 100 mV/div, averaging on.
23. Adjust the vertical and horizontal positioning to place the rising edge of the signal on the second vertical and center horizontal graticule lines.
24. Use the oscilloscope measurement capability to display rise time. Rise time is determined from the 10% and 90% amplitude points on the waveform. Record the rise time as t_{s+p} .
25. Calculate the probe rise time using the following formula:

$$t_p = \sqrt{t_{(s+p)}^2 - t_s^2}$$

26. Record the calculated probe rise time on the test record.

Rise Time Check at 2.5X Attenuation

The TDR output levels of the 80E08 module must be attenuated when checking the 2.5X attenuation setting on the probe. The attenuators add some delay and a small bandwidth reduction to the test system, so a new system time, t_s , must be measured to accurately calculate the probe rise time.

1. Disconnect the matched SMA cables from the TDR outputs.
2. Install inline 5X attenuators on the TDR outputs. (You will need to set the step offset to 25 mV and vertical scale to 10 mV/div. in the procedure).
3. Measure a new system time by repeating steps 1 through 16 of the 12.5X attenuation check.
4. Remove the TekConnect-to-SMA adapter from the test setup.
5. Connect the probe to the 80A03 TekConnect probe interface.
6. Connect the matched SMA cables to the probe SMA inputs and the inline 5X attenuators on the TDR outputs.
7. Set the attenuation on the probe to 2.5X and set the vertical scale to 20 mV/div, averaging on.
8. Repeat steps 21 through 25 for the 2.5X attenuation setting.
9. Record the calculated probe rise time on the test record.

Table 9: Test Record

Probe Model:

Serial Number:

Certificate Number:

Temperature:

RH %:

Date of Calibration:


Technician:

| Performance test | | Minimum | Measured | Maximum |
|------------------------------------|----------------|-------------|-------------------|--------------|
| Differential mode input resistance | | 98 Ω | | 102 Ω |
| Termination voltage accuracy | | | | |
| Ext Mode | Vin @ 0.000 V | Vin - 2 mV | Vin_____Vout_____ | Vin + 2 mV |
| | Vin @ +2.500 V | Vin - 7 mV | Vin_____Vout_____ | Vin + 7 mV |
| | Vin @ -2.500 V | Vin - 7 mV | Vin_____Vout_____ | Vin + 7 mV |
| Int Mode | Vin @ 0.000 V | -0.002 V | Vout | +0.002 V |
| | Vin @ +2.500 V | +2.4905 V | Vout | +2.5095 V |
| | Vin @ -2.500 V | -2.4905 V | Vout | -2.5095 V |
| Auto Mode | Vin @ 0.000 V | Vin - 20 mV | Vin_____Vout_____ | Vin + 20 mV |
| | Vin @ +2.500 V | Vin - 82 mV | Vin_____Vout_____ | Vin + 82 mV |
| | Vin @ -2.500 V | Vin - 82 mV | Vin_____Vout_____ | Vin + 82 mV |
| Output offset zero | 2.5X | -2.5 mV | | +2.5 mV |
| | 12.5X | -2.5 mV | | +2.5 mV |
| DC gain accuracy | 2.5X | 0.392 | | 0.408 |
| | 12.5X | 0.0784 | | 0.0816 |
| Differential rise time | 2.5X | NA | | 40 ps |
| | 12.5X | NA | | 40 ps |

Optional Accessories

The optional accessories that you can order for the P7313SMA differential probe are listed below. (See Table 10.)

Table 10: Optional accessories

| Description | Accessory |
|--|--|
| <p>Phase adjuster. Use two phase adjusters if you need to bring the skew between inputs to 1 ps or less because of skew in the device under test differential signal path. (See page 19, <i>Adjusting Cable Skew</i>.)The phase adjuster has a 25 ps adjustment range.</p> <p>The matched-delay SMA cables that come with your probe have a ≤ 1 ps skew at the cable ends.</p> <p>Tektronix part number: 015-0708-XX (package of 1)</p> |  |
| <p>80A03. The 80A03 TekConnect Probe Interface Module is an adapter that allows you to use TekConnect probes with CSA8000 and TDS8000 Series sampling oscilloscopes and 80E0X sampling modules.</p> <p>The interface contains an enclosure that houses a compartment for one 80E0X electrical sampling module and two TekConnect probe inputs. The interface routes the probe signal outputs through SMA connectors on the front panel. Semi-rigid SMA cables link the probe outputs to the 80E0X module inputs.</p> <p>The 80A03 Interface Module is required to complete a performance verification of the probe.</p> |  |

Options

These options are available when ordering the P7313SMA probe:

- Option D1-Calibration Data Report
- Option CA1-A single calibration event or coverage for the designated calibration interval, whichever comes first.
- Option D3-Calibration Data Report, 3 years (with Option C3)
- Option C3-Calibration Service 3 years
- Option D5-Calibration Data Report, 5 years (with Option C5)
- Option C5-Calibration Service 5 years
- Option R3-Repair Service 3 years
- Option R5-Repair Service 5 years

Maintenance

This section contains maintenance information for the P7313SMA differential probe.

Inspection and Cleaning

Protect the probe from adverse weather conditions. The probe is not waterproof.



CAUTION. To prevent damage to the probe, do not expose it to sprays, liquids, or solvents. Do not use chemical cleaning agents; they may damage the probe. Avoid using chemicals that contain benzine, benzene, toluene, xylene, acetone, or similar solvents.

Clean the exterior surfaces of the probe with a dry, lint-free cloth or a soft-bristle brush. If dirt remains, use a soft cloth or swab dampened with a 75% isopropyl alcohol solution. A swab is useful for cleaning narrow spaces on the probe. Do not use abrasive compounds on any part of the probe.



CAUTION. To prevent damage to the probe, avoid getting moisture inside the probe during exterior cleaning, and use only enough solution to dampen the swab or cloth. Use a 75% isopropyl alcohol solution as a cleanser, and rinse with deionized water.

Replacement Parts

Due to the sophisticated design of the P7313SMA differential probe, there are no user replaceable parts within the probe. Refer to the *Quick Start User Manual* for a list of replaceable accessories for your probe.

If your probe does not meet the specifications tested in the Performance Verification, you can send the probe to Tektronix for repair. Follow the procedure below to prevent damage to the probe during shipping.

Preparation for Shipment

If the original packaging is unfit for use or not available, use the following packaging guidelines:

1. Use a corrugated cardboard shipping carton having inside dimensions at least one inch greater than the probe dimensions. The box should have a carton test strength of at least 200 pounds.
2. Put the probe into an antistatic bag or wrap to protect it from dampness.
3. Place the probe into the box and stabilize it with light packing material.
4. Seal the carton with shipping tape.
5. Refer to *Contacting Tektronix* on the copyright page for the shipping address.