



# **4 Series MSO MS044, MS046, MS044B and MS046B**

## **Specifications and Performance Verification**

**Warning:** The servicing instructions are for use by qualified personnel only. To avoid personal injury, do not perform any servicing unless you are qualified to do so. Refer to all safety summaries prior to performing service.

Revision E

**Register now!**  
**Click the following link to protect your product.**  
**[tek.com/register](https://tek.com/register)**



077-1546-07 April 2025

Copyright © 2025, Tektronix. 2025 All rights reserved. Licensed software products are owned by Tektronix or its subsidiaries or suppliers, and are protected by national copyright laws and international treaty provisions. Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specifications and price change privileges reserved. All other trade names referenced are the service marks, trademarks, or registered trademarks of their respective companies.

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

Tektronix, Inc.  
14150 SW Karl Braun Drive  
P.O. Box 500  
Beaverton, OR 97077  
US

For product information, sales, service, and technical support visit [tek.com](https://www.tek.com) to find contacts in your area. For warranty information visit [tek.com/warranty](https://www.tek.com/warranty).

# Contents

List of Figures.....	5
List of Tables.....	6
Important safety information.....	7
General safety summary.....	7
To avoid fire or personal injury.....	7
Probes and test leads.....	9
Service safety summary.....	9
Terms in this manual.....	10
Terms on the product.....	10
Symbols on the product.....	10
Specifications.....	11
Analog channel input and vertical specification.....	11
Timebase system.....	19
Trigger system.....	21
Serial Trigger specifications.....	24
Digital acquisition system.....	24
Digital volt meter (DVM).....	24
Trigger frequency counter.....	24
Arbitrary Function Generator system.....	25
Display system.....	27
Processor system.....	27
Input/Output port specifications.....	28
Data storage specifications.....	29
Power supply system.....	32
Safety characteristics.....	32
Environmental specifications.....	32
Mechanical specifications.....	33
Performance verification procedures.....	34
Test record.....	35
Input Impedance test record.....	35
DC Gain Accuracy test record.....	36
DC Offset Accuracy test record.....	42
Analog Bandwidth test record.....	44
Random Noise High Res acquisition mode test record.....	74
Long term sample rate through AFG DC offset accuracy test records.....	109
Performance tests.....	117
Prerequisites.....	117
Self test.....	118
Check input impedance.....	119
Check DC gain accuracy.....	120
Check DC offset accuracy.....	122
Check analog bandwidth.....	124
Check random noise.....	125
Check long term sample rate.....	127

Check digital threshold accuracy.....	128
Check AUX Out output voltage levels.....	129
Check DVM voltage accuracy (DC).....	131
Check DVM voltage accuracy (AC).....	132
Check trigger frequency accuracy and maximum input frequency.....	132
Check AFG sine and ramp frequency accuracy.....	134
Check AFG square and pulse frequency accuracy.....	135
Check AFG signal amplitude accuracy.....	136
Check AFG DC offset accuracy.....	137

---

## List of Figures

Figure 1: Frequency/period test.....	134
Figure 2: Frequency/period test.....	135
Figure 3: 50 $\Omega$ terminator accuracy.....	136
Figure 4: Amplitude test.....	136
Figure 5: 50 $\Omega$ terminator accuracy.....	137
Figure 6: DC offset tests.....	138

## List of Tables

Table 1: Expected gain worksheet.....	121
Table 2: CF (Calibration Factor) = $1.414 \times ((50 / \text{Measurement } \Omega) + 1)$ .....	136
Table 3: CF (Calibration Factor) = $0.5 \times ((50 / \text{Measurement } \Omega) + 1)$ .....	137

# Important safety information

This manual contains information and warnings that must be followed by the user for safe operation and to keep the product in a safe condition.

To safely perform service on this product, see the *Service safety summary* that follows the *General safety summary*.

## General safety summary

Use the product only as specified. Review the following safety precautions to avoid injury and prevent damage to this product or any products connected to it. Carefully read all instructions. Retain these instructions for future reference.

This product shall be used in accordance with local and national codes.

For correct and safe operation of the product, it is essential that you follow generally accepted safety procedures in addition to the safety precautions specified in this manual.

The product is designed to be used by trained personnel only.

Only qualified personnel who are aware of the hazards involved should remove the cover for repair, maintenance, or adjustment.

Before use, always check the product with a known source to be sure it is operating correctly.

This product is not intended for detection of hazardous voltages.

Use personal protective equipment to prevent shock and arc blast injury where hazardous live conductors are exposed.

While using this product, you may need to access other parts of a larger system. Read the safety sections of the other component manuals for warnings and cautions related to operating the system.

When incorporating this equipment into a system, the safety of that system is the responsibility of the assembler of the system.

## To avoid fire or personal injury

### Use proper power cord

Use only the power cord specified for this product and certified for the country of use. Do not use the provided power cord for other products.

### Ground the product

This product is grounded through the grounding conductor of the power cord. To avoid electric shock, the grounding conductor must be connected to earth ground. Before making connections to the input or output terminals of the product, ensure that the product is properly grounded. Do not disable the power cord grounding connection.

### Power disconnect

The power cord disconnects the product from the power source. See instructions for the location. Do not position the equipment so that it is difficult to operate the power cord; it must remain accessible to the user at all times to allow for quick disconnection if needed.

### Connect and disconnect properly

Do not connect or disconnect probes or test leads while they are connected to a voltage source.

Use only insulated voltage probes, test leads, and adapters supplied with the product, or indicated by Tektronix to be suitable for the product.

### **Observe all terminal ratings**

To avoid fire or shock hazard, observe all rating and markings on the product. Consult the product manual for further ratings information before making connections to the product.

Do not exceed the Measurement Category (CAT) rating and voltage or current rating of the lowest rated individual component of a product, probe, or accessory. Use caution when using 1:1 test leads because the probe tip voltage is directly transmitted to the product.

Do not apply a potential to any terminal, including the common terminal, that exceeds the maximum rating of that terminal.

Do not float the common terminal above the rated voltage for that terminal.

The measurement terminals on this product are not rated for connection to Category III or IV circuits.

### **Do not operate without covers**

Do not operate this product with covers or panels removed, or with the case open. Hazardous voltage exposure is possible.

### **Avoid exposed circuitry**

Do not touch exposed connections and components when power is present.

### **Do not operate with suspected failures**

If you suspect that there is damage to this product, have it inspected by qualified service personnel.

Disable the product if it is damaged. Do not use the product if it is damaged or operates incorrectly. If in doubt about safety of the product, turn it off and disconnect the power cord. Clearly mark the product to prevent its further operation.

Before use, inspect voltage probes, test leads, and accessories for mechanical damage and replace when damaged. Do not use probes or test leads if they are damaged, if there is exposed metal, or if a wear indicator shows.

Examine the exterior of the product before you use it. Look for cracks or missing pieces.

Use only specified replacement parts.

### **Do not operate in wet/damp conditions**

Be aware that condensation may occur if a unit is moved from a cold to a warm environment.

### **Do not operate in an explosive atmosphere**

### **Keep product surfaces clean and dry**

Remove the input signals before you clean the product.

### **Provide proper ventilation**

Refer to the installation instructions in the manual for details on installing the product so it has proper ventilation.

Slots and openings are provided for ventilation and should never be covered or otherwise obstructed. Do not push objects into any of the openings.

### **Provide a safe working environment**

Always place the product in a location convenient for viewing the display and indicators.

Avoid improper or prolonged use of keyboards, pointers, and button pads. Improper or prolonged keyboard or pointer use may result in serious injury.

Be sure your work area meets applicable ergonomic standards. Consult with an ergonomics professional to avoid stress injuries.



Use care when lifting and carrying the product. This product is provided with a handle or handles for lifting and carrying.

Use only the Tektronix rackmount hardware specified for this product.

## Probes and test leads

Before connecting probes or test leads, connect the power cord from the power connector to a properly grounded power outlet.

Keep fingers behind the protective barrier, protective finger guard, or tactile indicator on the probes. Remove all probes, test leads and accessories that are not in use.

Use only correct Measurement Category (CAT), voltage, temperature, altitude, and amperage rated probes, test leads, and adapters for any measurement.

## Beware of high voltages

Understand the voltage ratings for the probe you are using and do not exceed those ratings. Two ratings are important to know and understand:

- The maximum measurement voltage from the probe tip to the probe reference lead.
- The maximum floating voltage from the probe reference lead to earth ground.

These two voltage ratings depend on the probe and your application. Refer to the Specifications section of the manual for more information.



**WARNING:** To prevent electrical shock, do not exceed the maximum measurement or maximum floating voltage for the oscilloscope input BNC connector, probe tip, or probe reference lead.

## Connect and disconnect properly

Connect the probe output to the measurement product before connecting the probe to the circuit under test. Connect the probe reference lead to the circuit under test before connecting the probe input. Disconnect the probe input and the probe reference lead from the circuit under test before disconnecting the probe from the measurement product.

De-energize the circuit under test before connecting or disconnecting the current probe.

Connect the probe reference lead to earth ground only.

Do not connect a current probe to any wire that carries voltages or frequencies above the current probe voltage rating.

## Inspect the probe and accessories

Before each use, inspect probe and accessories for damage (cuts, tears, or defects in the probe body, accessories, or cable jacket). Do not use if damaged.

## Service safety summary

The *Service safety summary* section contains additional information required to safely perform service on the product. Only qualified personnel should perform service procedures. Read this *Service safety summary* and the *General safety summary* before performing any service procedures.

## To avoid electric shock

Do not touch exposed connections.

## Do not service alone

Do not perform internal service or adjustments of this product unless another person capable of rendering first aid and resuscitation is present.

## Disconnect power

To avoid electric shock, switch off the product power and disconnect the power cord from the mains power before removing any covers or panels, or opening the case for servicing.

## Use care when servicing with power on

Dangerous voltages or currents may exist in this product. Disconnect power, remove battery (if applicable), and disconnect test leads before removing protective panels, soldering, or replacing components.

## Verify safety after repair

Always recheck ground continuity and mains dielectric strength after performing a repair.

## Terms in this manual

These terms may appear in this manual:



**WARNING:** Warning statements identify conditions or practices that could result in injury or loss of life.



**CAUTION:** Caution statements identify conditions or practices that could result in damage to this product or other property.

## Terms on the product

These terms may appear on the product:

- DANGER indicates an injury hazard immediately accessible as you read the marking.
- WARNING indicates an injury hazard not immediately accessible as you read the marking.
- CAUTION indicates a hazard to property including the product.

## Symbols on the product



When this symbol is marked on the product, be sure to consult the manual to find out the nature of the potential hazards and any actions which have to be taken to avoid them. (This symbol may also be used to refer the user to ratings in the manual.)

The following symbols(s) may appear on the product.



CAUTION: Refer to Manual



Protective Ground (Earth) Terminal



Chassis Ground



Standby



Functional Earth Terminal

# Specifications

This chapter contains specifications for the instrument. All specifications are typical unless noted as guaranteed. Typical specifications are provided for your convenience but are not guaranteed. Specifications that are marked with the ✓ symbol are guaranteed and checked in Performance Verification.

To meet specifications, these conditions must first be met:

- The instrument must have been calibrated in an ambient temperature between 18 °C and 28 °C (64 °F and 82 °F).
- The instrument must be operating within the environmental limits described in this manual.
- The instrument must be powered from a source that meets the specifications.
- The instrument must have been operating continuously for at least 20 minutes within the specified operating temperature range.
- You must perform the Signal path compensation procedure after the warmup period. See the Signal path compensation procedure for how to perform signal path compensation. If the ambient temperature changes more than 5 °C (9 °F), repeat the procedure.
- The measurement system is powered from a TekVPI compatible oscilloscope.

Warranted specifications describe guaranteed performance with tolerance limits or certain type-tested requirements.

## Analog channel input and vertical specification

<b>Number of input channels</b>	4 analog channel model: 4 BNC 6 analog channel model: 6 BNC
<b>Input coupling</b>	DC, AC
<b>Input resistance selection</b>	1 M $\Omega$ or 50 $\Omega$
<b>✓ Input impedance 1 M<math>\Omega</math> DC coupled</b>	1 M $\Omega$ $\pm$ 1%
<b>Input capacitance 1 M<math>\Omega</math> DC coupled, typical</b>	13 pF $\pm$ 1.5 pF
<b>✓ Input impedance 50 <math>\Omega</math>, DC coupled</b>	<b>MSO44, MSO46:</b> 50 $\Omega$ $\pm$ 1% (VSWR $\leq$ 1.5:1, typical) <b>MSO44B, MSO46B:</b> 50 $\Omega$ $\pm$ 1% (VSWR $\leq$ 1.5:1, typical for frequencies <1GHz, $\leq$ 2.0:1 for frequencies equal to or above 1GHz)
<b>Maximum input voltage, 1 M<math>\Omega</math></b>	300 V <sub>RMS</sub> at the BNC  Derate at 20 dB/decade between 4.5 MHz and 45 MHz; derate 14 dB/decade between 45 MHz and 450 MHz. Above 450 MHz, 5.5 V <sub>RMS</sub>  Maximum peak input voltage at the BNC: $\pm$ 425 V
<b>Maximum input voltage, 50 <math>\Omega</math></b>	5 V <sub>RMS</sub> , with peaks $\leq$ $\pm$ 20 V (DF $\leq$ 6.25%)
<b>Number of Digitized Bits</b>	8 bits at 6.25 GS/s 12 bits at 3.125 GS/s 13 bits at 1.25 GS/s 14 bits at 625 MS/s

15 bits at 250 MS/s

16 bits at 125 MS/s

Displayed vertically with 25 digitization levels (DL) for 8-bit and 400 digitization levels for 12-bit per division, 10.24 divisions dynamic range. DL is the abbreviation for digitization level. A DL is the smallest voltage level change that can be resolved by an 8-bit A-D Converter. This value is also known as an LSB (least significant bit).

**Sensitivity range, coarse**

**1 M $\Omega$**  500  $\mu$ V/div to 10 V/div in a 1-2-5 sequence

**50  $\Omega$**  500  $\mu$ V/div to 1 V/div in a 1-2-5 sequence

500  $\mu$ V/div is a 2X digital zoom of 1 mV/div or a 4x digital zoom of 2 mV/div, depending on the instrument bandwidth configuration

**Sensitivity range, fine**

**1 M $\Omega$**  Allows continuous adjustment from 500  $\mu$ V/div to 10 V/div

**50  $\Omega$**  Allows continuous adjustment from 500  $\mu$ V/div to 1 V/div

**Sensitivity resolution, fine**  $\leq$ 1% of current setting

**✓ DC gain accuracy**

**Step Gain, 50  $\Omega$**   $\pm$ 1.0%, ( $\pm$ 2.5% at 1 mV/div and 500  $\mu$ V/div settings), de-rated at 0.100%/  $^{\circ}$ C above 30  $^{\circ}$ C

**Step Gain, 1 M $\Omega$**   $\pm$ 1.0%, ( $\pm$ 2.0% at 1 mV/div and 500  $\mu$ V/div settings), de-rated at 0.100%/  $^{\circ}$ C above 30  $^{\circ}$ C

**Variable gain**  $\pm$ 1.5%, derated at 0.100%/  $^{\circ}$ C above 30  $^{\circ}$ C.

500  $\mu$ V/div is a 2X digital zoom of 1 mV/div or a 4x digital zoom of 2 mV/div, depending on the instrument bandwidth configuration. As such, it is guaranteed by testing the non-zoomed setting.

**Offset ranges, maximum** Input signal cannot exceed maximum input voltage for the 50  $\Omega$  input path.

Volts/div setting	Maximum offset range, 50 $\Omega$ input
500 $\mu$ V/div - 99 mV/div	$\pm$ 1 V
100 mV/div - 1 V/div	$\pm$ 10 V

Volts/div setting	Maximum offset range, 1 M $\Omega$ input
500 $\mu$ V/div - 63 mV/div	$\pm$ 1 V
64 mV/div - 999 mV/div	$\pm$ 10 V
1 V/div - 10 V/div	$\pm$ 100 V

500  $\mu$ V/div is a 2X digital zoom of 1 mV/div or a 4x digital zoom of 2 mV/div, depending on the instrument bandwidth configuration. As such, it is guaranteed by testing the non-zoomed setting.

**Position range**  $\pm$ 5 divisions

✓ **DC Offset accuracy**  $\pm(0.010 \times |\text{offset} - \text{position}| + \text{DC balance})$

DC Balance is 0.2 div (0.4 div in 500  $\mu\text{V}/\text{div}$ )

**DC voltage measurement accuracy, Average acquisition mode**

Measurement Type	DC Accuracy (In Volts)
Average of $\geq 16$ waveforms	$\pm((\text{DC Gain Accuracy}) *  \text{reading} - (\text{offset} - \text{position})  + \text{Offset Accuracy} + 0.1 * \text{V}/\text{div setting})$
Delta volts between any two averages of $\geq 16$ waveforms acquired with the same oscilloscope setup and ambient conditions	$\pm(\text{DC Gain Accuracy} *  \text{reading}  + 0.05 \text{ div})$

**Bandwidth selections**

50  $\Omega$ : 20 MHz, 250 MHz, and the full bandwidth value of your model

1 M $\Omega$ : 20 MHz, 250 MHz, 350 MHz, 500 MHz

350 MHz models cannot be configured to 500 MHz in 1 M $\Omega$  mode

✓ **Analog bandwidth 50  $\Omega$  DC coupled**

**1.5 GHz models**

Volts/Div Setting	Bandwidth
1 mV/div - 1 V/div	DC - 1.50 GHz
500 $\mu\text{V}/\text{div}$ - 995 $\mu\text{V}/\text{div}$	DC - 250 MHz

**1 GHz models**

Volts/Div Setting	Bandwidth
1 mV/div - 1 V/div	DC - 1.00 GHz
500 $\mu\text{V}/\text{div}$ - 995 $\mu\text{V}/\text{div}$	DC - 250 MHz

**500 MHz models**

Volts/Div Setting	Bandwidth
1 mV/div - 1 V/div	DC - 500 MHz
500 $\mu\text{V}/\text{div}$ - 995 $\mu\text{V}/\text{div}$	DC - 250 MHz

**350 MHz models**

Volts/Div Setting	Bandwidth
1 mV/div - 1 V/div	DC - 350 MHz
500 $\mu\text{V}/\text{div}$ - 995 $\mu\text{V}/\text{div}$	DC - 250 MHz

**200 MHz models**

Volts/Div Setting	Bandwidth
1 mV/div - 1 V/div	DC - 200 MHz
500 $\mu\text{V}/\text{div}$ - 995 $\mu\text{V}/\text{div}$	DC - 200 MHz

**Analog bandwidth, 1 M $\Omega$ , typical**

**All model bandwidths except 350 MHz, 200 MHz**

The limits are for ambient temperature of  $\leq 30$  °C and the bandwidth selection set to FULL. Reduce the upper bandwidth frequency by 1% for each °C above 30 °C.

Volts/Div Setting	Bandwidth
1 mV/div - 10 V/div	DC - 500 MHz
500 $\mu$ V/div - 995 $\mu$ V/div	DC - 250 MHz

**350 MHz models**

Volts/Div Setting	Bandwidth
1 mV/div - 10 V/div	DC - 350 MHz
500 $\mu$ V/div - 995 $\mu$ V/div	DC - 250 MHz

**200 MHz models**

Volts/Div Setting	Bandwidth
1 mV/div - 10 V/div	DC - 200 MHz
500 $\mu$ V/div - 995 $\mu$ V/div	DC - 200 MHz

**Analog bandwidth with TPP0500, TPP1000 and TPP0250 probes, typical**

The limits are for ambient temperature of  $\leq 30$  °C and the bandwidth selection set to FULL. Reduce the upper bandwidth frequency by 1% for each °C above 30 °C.

Instrument	Volts/Div Setting	Bandwidth
1.5 GHz, 1 GHz	5 mV/div - 100 V/div	DC - 1 GHz (TPP1000 Probe)
500 MHz	5 mV/div - 100 V/div	DC - 500 MHz (TPP0500 Probe)
350 MHz	5 mV/div - 100 V/div	DC - 350 MHz (TPP0500 Probe)
200 MHz	5 mV/div - 100 V/div	DC - 200 MHz (TPP0250 Probe)

**Lower frequency limit, AC coupled, typical**

<10 Hz when AC 1 M $\Omega$  coupled. The AC coupled lower frequency limits are reduced by a factor of 10 (<1 Hz) when 10X passive probes are used.

**Upper frequency limit, 250 MHz bandwidth limited, typical**

250 MHz,  $\pm 25\%$

**Upper frequency limit, 20 MHz bandwidth limited, typical**

20 MHz,  $\pm 25\%$

**Calculated rise time, typical**

Model	50 $\Omega$	TP1000 Probe	TPP0500 Probe	TPP0250 Probe
	500 $\mu$ V-1 V	5 mV-10 V	5 mV-10 V	5 mV-10 V
1.5 GHz	333ps	450ps	900ps	1.8ns
1 GHz	450ps	450ps	900ps	1.8ns
500 MHz	900ps	900ps	900ps	1.8ns
350 MHz	1.3ns	1.3ns	1.3ns	1.8ns
200 MHz	2.3ns	2.3ns	2.3ns	2.3ns

**Peak Detect or Envelope mode** Minimum pulse width is >640 ps (6.25 GS/s)  
**pulse response, typical**

**Effective bits (ENOB), typical**

Typical effective bits for a 9-division p-p sine-wave input, 50 mV/div, 50-Ω

**Sample mode, 50 Ω, 50 mV/div**

Bandwidth	Input frequency	ENOB at 6.25 GS/s
1.5 GHz	10 MHz	6.80
1.5 GHz	300 MHz	6.80
1 GHz	10 MHz	7.10
1 GHz	300 MHz	7.10
500 MHz	10 MHz	7.40
500 MHz	150 MHz	7.40
350 MHz	10 MHz	7.60
350 MHz	100 MHz	7.60
250 MHz	10 MHz	7.60
250 MHz	100 MHz	7.60
200 MHz	10 MHz	7.60
200 MHz	100 MHz	7.60
20 MHz	10 MHz	7.70

**High Res mode, 50 Ω, 50 mV/div**

Bandwidth	Input frequency	ENOB at 6.25 GS/s
1.5 GHz	10 MHz	7.10
1.5 GHz	300 MHz	7.10
1 GHz	10 MHz	7.60
1 GHz	300 MHz	7.60
500 MHz	10 MHz	7.90
500 MHz	150 MHz	7.90
350 MHz	10 MHz	8.20
350 MHz	100 MHz	8.20
250 MHz	10 MHz	8.20
250 MHz	100 MHz	8.20
200 MHz	10 MHz	8.20
200 MHz	100 MHz	8.20
20 MHz	10 MHz	8.90

**Random noise, Sample and High Res Acquisition modes, 50 Ω and 1 MΩ, 6.25 Gs/s**

✓ 1.5 GHz models,  
Sample mode (RMS), 50 Ω

V/div	1.5 GHz
1 mV/div	635 μV
2 mV/div	635 μV
5 mV/div	817 μV
10 mV/div	843 μV
20 mV/div	920 μV
50 mV/div	1.582 mV
100 mV/div	3.686 mV
1 V/div	23.753 mV

MSO44 and MSO46,  
Sample mode (RMS), 50 Ω,  
typical

V/div	1.5 GHz	1 GHz	500 MHz	350 MHz	250/200 MHz	20 MHz
1 mV/div	490 μV	300 μV	220 μV	145 μV	120 μV	80 μV
2 mV/div	490 μV	350 μV	220 μV	150 μV	130 μV	80 μV
5 mV/div	630 μV	380 μV	230 μV	175 μV	160 μV	110 μV
10 mV/div	650 μV	400 μV	280 μV	220 μV	215 μV	155 μV
20 mV/div	710 μV	510 μV	410 μV	340 μV	340 μV	260 μV
50 mV/div	1.220 mV	980 μV	890 μV	760 μV	760 μV	630 μV
100 mV/div	2.84 mV	2.23 mV	1.93 mV	1.61 mV	1.61 mV	1.25 mV
1 V/div	18.3 mV	19.0 mV	17.3 mV	15.0 mV	15.0 mV	12.5 mV

MSO44B and MSO46B,  
Sample mode (RMS), 50 Ω,  
typical

V/div	1.5 GHz	1 GHz	500 MHz	350 MHz	250/200 MHz	20 MHz
1 mV/div	520 μV	320 μV	210 μV	150 μV	120 μV	80 μV
2 mV/div	520 μV	350 μV	220 μV	150 μV	120 μV	80 μV
5 mV/div	620 μV	380 μV	230 μV	175 μV	160 μV	110 μV
10 mV/div	620 μV	400 μV	270 μV	220 μV	215 μV	180 μV
20 mV/div	720 μV	510 μV	410 μV	360 μV	370 μV	320 μV
50 mV/div	1.30 mV	1.05 mV	930 μV	880 μV	900 μV	700 μV
100 mV/div	3.00 mV	2.23 mV	1.93 mV	1.74 mV	1.78 mV	1.45 mV
1 V/div	21.0 mV	19.3 mV	18.1 mV	17.5 mV	17.6 mV	14.0 mV

✓ All models except  
1.5 GHz, High Res mode  
(RMS), 50 Ω

V/div	1 GHz	500 MHz	350 MHz	250/200 MHz	20 MHz
1 mV/div	336 μV	259 μV	194 μV	161 μV	96 μV
2 mV/div	363 μV	259 μV	194 μV	161 μV	96 μV
5 mV/div	394 μV	304 μV	239 μV	174 μV	96 μV
10 mV/div	434 μV	356 μV	284 μV	206 μV	103 μV
20 mV/div	551 μV	466 μV	349 μV	298 μV	141 μV

Table continued...



V/div	1 GHz	500 MHz	350 MHz	250/200 MHz	20 MHz
50 mV/div	1.038 mV	1.038 mV	739 $\mu$ V	596 $\mu$ V	259 $\mu$ V
100 mV/div	2.102 mV	1.596 mV	1.349 mV	1.349 mV	609 $\mu$ V
1 V/div	16.874 mV	12.850 mV	11.617 mV	11.617 mV	4.906 mV

**MSO44 and MSO46, except  
1.5 GHz, High Res mode  
(RMS), 50  $\Omega$ , typical**

V/div	1 GHz	500 MHz	350 MHz	250/200 MHz	20 MHz
1 mV/div	260 $\mu$ V	200 $\mu$ V	150 $\mu$ V	125 $\mu$ V	75 $\mu$ V
2 mV/div	280 $\mu$ V	200 $\mu$ V	150 $\mu$ V	125 $\mu$ V	75 $\mu$ V
5 mV/div	305 $\mu$ V	235 $\mu$ V	185 $\mu$ V	135 $\mu$ V	75 $\mu$ V
10 mV/div	335 $\mu$ V	275 $\mu$ V	220 $\mu$ V	160 $\mu$ V	80 $\mu$ V
20 mV/div	425 $\mu$ V	360 $\mu$ V	270 $\mu$ V	230 $\mu$ V	110 $\mu$ V
50 mV/div	800 $\mu$ V	800 $\mu$ V	570 $\mu$ V	460 $\mu$ V	200 $\mu$ V
100 mV/div	1.62 mV	1.23 mV	1.04 mV	1.04 mV	480 $\mu$ V
1 V/div	13.0 mV	9.90 mV	8.95 mV	8.95 mV	3.78 mV

**MSO44B and MSO46B,  
except 1.5 GHz, High Res  
mode (RMS), 50  $\Omega$ , typical**

V/div	1 GHz	500 MHz	350 MHz	250/200 MHz	20 MHz
1 mV/div	280 $\mu$ V	210 $\mu$ V	150 $\mu$ V	125 $\mu$ V	75 $\mu$ V
2 mV/div	280 $\mu$ V	210 $\mu$ V	150 $\mu$ V	125 $\mu$ V	75 $\mu$ V
5 mV/div	300 $\mu$ V	230 $\mu$ V	185 $\mu$ V	135 $\mu$ V	75 $\mu$ V
10 mV/div	330 $\mu$ V	260 $\mu$ V	220 $\mu$ V	160 $\mu$ V	80 $\mu$ V
20 mV/div	420 $\mu$ V	350 $\mu$ V	270 $\mu$ V	230 $\mu$ V	110 $\mu$ V
50 mV/div	800 $\mu$ V	780 $\mu$ V	570 $\mu$ V	460 $\mu$ V	200 $\mu$ V
100 mV/div	1.65 mV	1.29 mV	1.04 mV	1.04 mV	480 $\mu$ V
1 V/div	13.0 mV	10.0 mV	8.95 mV	8.95 mV	3.78 mV

**MSO44 and MSO46,  
Sample mode (RMS), 1 M $\Omega$ ,  
typical**

V/div	500 MHz	350 MHz	250/200 MHz	20 MHz
1 mV/div	210 $\mu$ V	140 $\mu$ V	120 $\mu$ V	78 $\mu$ V
2 mV/div	210 $\mu$ V	140 $\mu$ V	120 $\mu$ V	78 $\mu$ V
5 mV/div	230 $\mu$ V	160 $\mu$ V	135 $\mu$ V	96 $\mu$ V
10 mV/div	270 $\mu$ V	200 $\mu$ V	190 $\mu$ V	135 $\mu$ V
20 mV/div	370 $\mu$ V	300 $\mu$ V	300 $\mu$ V	240 $\mu$ V
50 mV/div	760 $\mu$ V	600 $\mu$ V	650 $\mu$ V	750 $\mu$ V
100 mV/div	1.75 mV	1.350 mV	1.45 mV	1.22 mV
1 V/div	19.00 mV	15.25 mV	15.70 mV	11.20 mV

**MSO44B and MSO46B,  
Sample mode (RMS), 1 M $\Omega$ ,  
typical**

V/div	500 MHz	350 MHz	250/200 MHz	20 MHz
1 mV/div	220 $\mu$ V	150 $\mu$ V	120 $\mu$ V	75 $\mu$ V
2 mV/div	220 $\mu$ V	150 $\mu$ V	120 $\mu$ V	75 $\mu$ V
5 mV/div	230 $\mu$ V	170 $\mu$ V	135 $\mu$ V	100 $\mu$ V
10 mV/div	270 $\mu$ V	210 $\mu$ V	200 $\mu$ V	170 $\mu$ V
20 mV/div	370 $\mu$ V	300 $\mu$ V	300 $\mu$ V	240 $\mu$ V
50 mV/div	760 $\mu$ V	600 $\mu$ V	650 $\mu$ V	750 $\mu$ V
100 mV/div	1.75 mV	1.350 mV	1.45 mV	1.22 mV
1 V/div	19.00 mV	15.25 mV	15.70 mV	11.20 mV

**MSO44 and MSO46, High  
Res mode (RMS), 1 M $\Omega$ ,  
typical**

V/div	500 MHz	350 MHz	250/200 MHz	20 MHz
1 mV/div	200 $\mu$ V	140 $\mu$ V	120 $\mu$ V	75 $\mu$ V
2 mV/div	200 $\mu$ V	140 $\mu$ V	120 $\mu$ V	75 $\mu$ V
5 mV/div	210 $\mu$ V	150 $\mu$ V	130 $\mu$ V	75 $\mu$ V
10 mV/div	230 $\mu$ V	160 $\mu$ V	150 $\mu$ V	80 $\mu$ V
20 mV/div	280 $\mu$ V	200 $\mu$ V	200 $\mu$ V	100 $\mu$ V
50 mV/div	520 $\mu$ V	370 $\mu$ V	410 $\mu$ V	180 $\mu$ V
100 mV/div	1.24 mV	880 $\mu$ V	930 $\mu$ V	460 $\mu$ V
1 V/div	14.3 mV	10.20 mV	10.30 mV	5.45 mV

**MSO44B and MSO46B,  
High Res mode (RMS), 1  
M $\Omega$ , typical**

V/div	500 MHz	350 MHz	250/200 MHz	20 MHz
1 mV/div	200 $\mu$ V	150 $\mu$ V	120 $\mu$ V	70 $\mu$ V
2 mV/div	210 $\mu$ V	150 $\mu$ V	120 $\mu$ V	70 $\mu$ V
5 mV/div	220 $\mu$ V	160 $\mu$ V	130 $\mu$ V	70 $\mu$ V
10 mV/div	230 $\mu$ V	170 $\mu$ V	150 $\mu$ V	75 $\mu$ V
20 mV/div	300 $\mu$ V	230 $\mu$ V	220 $\mu$ V	100 $\mu$ V
50 mV/div	550 $\mu$ V	450 $\mu$ V	450 $\mu$ V	200 $\mu$ V
100 mV/div	1.35 mV	1.00 mV	1.03 mV	480 $\mu$ V
1 V/div	15.0 mV	11.5 mV	11.5 mV	5.80 mV

**✓ All models, High Res  
mode (RMS), 1 M $\Omega$**

V/div	500 MHz	350 MHz	250/200 MHz	20 MHz
1 mV/div	259 $\mu$ V	181 $\mu$ V	155 $\mu$ V	96 $\mu$ V
2 mV/div	259 $\mu$ V	181 $\mu$ V	155 $\mu$ V	96 $\mu$ V
5 mV/div	271 $\mu$ V	194 $\mu$ V	168 $\mu$ V	96 $\mu$ V
10 mV/div	298 $\mu$ V	206 $\mu$ V	194 $\mu$ V	103 $\mu$ V
20 mV/div	363 $\mu$ V	259 $\mu$ V	259 $\mu$ V	129 $\mu$ V

Table continued...

V/div	500 MHz	350 MHz	250/200 MHz	20 MHz
50 mV/div	674 $\mu$ V	479 $\mu$ V	531 $\mu$ V	233 $\mu$ V
100 mV/div	1.609 mV	1.141 mV	1.206 mV	596 $\mu$ V
1 V/div	18.561 mV	13.239 mV	13.369 mV	7.074 mV

**Delay between analog channels, full bandwidth, typical**

$\leq 100$  ps for any two channels with input impedance set to  $50 \Omega$ , DC coupling with equal Volts/div or above 10 mV/div

**Deskew range**

**MSO44, MSO46:** -125 ns to +125 ns with a resolution of 40 ps

**MSO44B, MSO46B:** -125 ns to +125 ns with a resolution of 40 ps (for Peak Detect and Envelope acquisition modes). -125 ns to +125 ns with a resolution of 1 ps (for all other acquisition modes).

**Crosstalk (channel isolation), typical**

$\geq 200:1$  up to the rated bandwidth for any two channels having equal Volts/div settings

**Total probe power**

TekVPI+ Compliant probe interfaces: (4 per MSO44, 6 per MSO46) and 1 TekVPI interface for Aux In  
MSO46: 80 W maximum (40 W maximum for channels 1-3, 40 W maximum for channels 4-6 and Aux In)  
MSO44: 80 W maximum (40 W maximum for channels 1-3, 40 W maximum for channel 4 and Aux In)

**Probe power per channel**

Voltage	Max Amperage	Voltage Tolerance
5 V	60 mA	$\pm 10\%$
12 V	1.67 A (20 W maximum software limit)	$\pm 10\%$

**TekVPI interconnect**

All analog channel inputs on the front panel conform to the TEKVPI specification.

## Timebase system

**Sample rate**

Max HW Capability	Number of Channels
6.25 GS/s	1-6

**Interpolated waveform rate range**

500 GS/sec, 250 GS/sec, 125 GS/sec, 62.5 GS/sec, 25 GS/sec, and 12.5 GS/sec

**Record length range**

**Standard**

1 k points to 31.25 M points in single sample increments

**Optional**

62.5 M points

**Seconds/Division range**

Model	1 K	10 K	100 K	1 M	10 M	31.25 M	62.5 M
MSO44/MSO46 Standard 31.25 M	200 ps - 64 s	2 ns - 640 s	20 ns - 1000 s	200 ns - 1000 s	2 μs - 1000 s	6.25 μs - 1000 s	N/A
MSO44/MSO46 Option 62.5 M	200 ps - 64 s	2 ns - 640 s	20 ns - 1000 s	200 ns - 1000 s	2 μs - 1000 s	6.25 μs - 1000 s	12.5 μs - 1000 s
MSO44B/MSO46B Standard 31.25 M	200 ps - 64 s	2 ns - 640 s	20 ns - 1000 s	200 ns - 1000 s	2 μs - 1000 s	6.25 μs - 1000 s	N/A
MSO44B/MSO46B Option 62.5 M	200 ps - 64 s	2 ns - 640 s	20 ns - 1000 s	200 ns - 1000 s	2 μs - 1000 s	6.25 μs - 1000 s	12.5 μs - 1000 s

**Maximum triggered acquisition rate, typical**

Analog or digital channels: single channel [Analog or Digital 8-bit channel] on screen, measurements and math turned off. >20 wfm/sec

FastAcq Update Rate (analog only): >500 K/second with one channel active and >100 K/second with all channels active.

Digital channel: >20/second with one channel (8-bits) active. There is no FastAcq for digital channels, but they do not slow down FastAcq for active analog channels.

**Aperture uncertainty**

$\leq 800 \text{ fs} + (10^{-11} * \text{Measurement Duration})_{\text{RMS}}$ , for measurements having duration  $\leq 100 \text{ ms}$

**✓ Timebase accuracy**

$\pm 2.5 \times 10^{-6}$  over any  $\geq 1 \text{ ms}$  time interval.

Description	Specification
Factory Tolerance	$\pm 5.0 \times 10^{-7}$ ; at calibration, 25 °C ambient, over any $\geq 1 \text{ ms}$ interval.
Temperature stability, typical	$\pm 5.0 \times 10^{-7}$ ; tested at operating temperatures.
Crystal aging	$\pm 1.5 \times 10^{-6}$ ; frequency tolerance change at 25 °C over a period of 1 year.

**Delta-time measurement accuracy, nominal**

The formulas to calculate the peak-to-peak or rms nominal delta-time measurement accuracy (DTA) for a given instrument setting and input signal is as follows (assumes insignificant signal content above Nyquist frequency):

$$DTA_{pp}(\text{typical}) = 10 \times \sqrt{\left(\frac{N}{SR_1}\right)^2 + \left(\frac{N}{SR_2}\right)^2 + \left(0.450 \text{ ps} + \left(1 \times 10^{-11} \times t_p\right)\right)^2} + TBA \times t_p$$

$$DTA_{\text{RMS}} = \sqrt{\left(\frac{N}{SR_1}\right)^2 + \left(\frac{N}{SR_2}\right)^2 + \left(0.450 \text{ ps} + \left(1 \times 10^{-11} \times t_p\right)\right)^2} + TBA \times t_p$$

Where:

N = input-referred guaranteed noise limit ( $V_{\text{RMS}}$ )

$SR_1$  = Slew Rate (1<sup>st</sup> Edge) around 1<sup>st</sup> point in measurement

$SR_2$  = Slew Rate (2<sup>nd</sup> Edge) around 2<sup>nd</sup> point in measurement

$t_p$  = delta-time measurement duration (sec)

TBA = timebase accuracy or Reference Frequency Error  $\pm 0.5$  ppm

*(Assumes insignificant error due to aliasing or over-drive.)*

The term under the square root sign is the stability and is due to TIE (Time Interval Error). The errors due to this term occur throughout a single-shot measurement. The second term is due to both the absolute center-frequency accuracy and the center-frequency stability of the timebase and varies between multiple single-shot measurements over the observation interval (the amount of time from the first single-shot measurement to the final single-shot measurement).



**Note:** The formulas assume negligible errors due to measurement interpolation, and apply only when the interpolated sample rate is 25 GS/s or higher.

## Trigger system

Trigger bandwidth (edge, pulse, and logic)

1.5 GHz models, Edge = 1.5 GHz

1.5 GHz models, Pulse and Logic = 1 GHz

1 GHz models = 1 GHz

500 MHz models = 500 MHz

350 MHz models = 350 MHz

200 MHz models = 200 MHz

Edge-type trigger sensitivity, DC coupled, typical

Path	Range	Specification
1 M $\Omega$ path (all models)	0.5 mV/div to 0.99 mV/div	4.5 div from DC to instrument bandwidth
	$\geq 1$ mV/div	The greater of 5 mV or 0.7 div
50 $\Omega$ path, all models		The greater of 5.6 mV or 0.7 div for frequencies between DC and 500 MHz or the instrument bandwidth (whichever is lower)
		The greater of 7 mV or 0.8 div for frequencies above 500 MHz (if applicable)

Trigger jitter, typical

$\leq 7$  pSRMS

Edge-type trigger sensitivity, not DC coupled, typical

Trigger Coupling	Typical Sensitivity
NOISE REJ	2.5 times the DC Coupled limits
HF REJ	1.0 times the DC Coupled limits from DC to 50 kHz. Attenuates signals above 50 kHz.
LF REJ	1.5 times the DC Coupled limits for frequencies above 50 kHz. Attenuates signals below 50 kHz.

**Logic-type triggering, minimum logic or rearm time, typical**

$t_{rise}$  is rise time of the instrument.

Triggering type	Pulse width	Rearm time	Time skew needed for 100% and no triggering
Logic	$160\text{ ps} + t_{rise}$	$160\text{ ps} + t_{rise}$	$>360\text{ ps} / <150\text{ ps}$
Time qualified logic	$320\text{ ps} + t_{rise}$	$320\text{ ps} + t_{rise}$	$>360\text{ ps} / <150\text{ ps}$

For Logic, time between channels refers to the length of time a logic state derived from more than one channel must exist to be recognized. For Events, the time is the minimum time between a main and delayed event that will be recognized if more than one channel is used.

**Minimum clock pulse widths for setup/hold time violation trigger, typical**

$t_{rise}$  is rise time of the instrument.

Minimum pulsewidth, clock active	Minimum pulsewidth, clock inactive
$320\text{ ps} + t_{rise}$	$320\text{ ps} + t_{rise}$

Active pulsewidth is the width of the clock pulse from its active edge (as defined in the Clock Edge menu item) to its inactive edge. Inactive pulsewidth is the width of the pulse from its inactive edge to its active edge.

**Setup/hold violation trigger, setup and hold time ranges, typical**

Feature	Min	Max
Setup Time	0 ns	20 s
Hold Time	0 ns	20 s
Setup + Hold Time	320 ps	22 s

Input coupling on clock and data channels must be the same.

For Setup Time, positive numbers mean a data transition before the clock.

For Hold Time, positive numbers mean a data transition after the clock edge.

Setup + Hold Time is the algebraic sum of the Setup Time and the Hold Time programmed by the user.

**Pulse type trigger, minimum pulse, rearm time, transition time**

Pulse class	Minimum pulse width	Minimum rearm time
Runt	$160\text{ ps} + t_{rise}$	$160\text{ ps} + t_{rise}$
Time-Qualified Runt	$160\text{ ps} + t_{rise}$	$160\text{ ps} + t_{rise}$
Width	$160\text{ ps} + t_{rise}$	$160\text{ ps} + t_{rise}$
Slew Rate (minimum transition time)	$160\text{ ps} + t_{rise}$	$160\text{ ps} + t_{rise}$

For trigger class width, pulse width refers to the width of the pulse being measured. Rearm time refers to the time between pulses.

For trigger class runt, pulse width refers to the width of the pulse being measured. Rearm time refers to the time between pulses.

For trigger class slew rate, pulse width refers to the delta time being measured. Rearm time refers to the time it takes the signal to cross the two trigger thresholds again.

$t_{rise}$  is rise time of the instrument.

Active pulsewidth is the width of the clock pulse from its active edge (as defined in the Clock Edge menu item) to its inactive edge

Inactive pulsewidth is the width of the pulse from its inactive edge to its active edge.

**Transition time trigger, delta time range** 160 ps to 20 s.

**Time range for glitch, pulse width, timeout, time-qualified runt, or time-qualified window triggering** 160 ps to 20 s.

**Time accuracy for pulse, glitch, timeout, or width triggering**

Time Range	Accuracy
320 ps to 500 ns	$\pm(160 \text{ ps} + (\text{Time-Base-Accuracy} * \text{Setting}))$
520 ns to 10 s	$\pm(160 \text{ ps} + (\text{Time-Base-Accuracy} * \text{Setting}))$

**B trigger after events, minimum pulse width and maximum event frequency, typical**

Minimum pulse width:  $160 \text{ ps} + t_{rise}$

Maximum event frequency: Instrument bandwidth.

$t_{rise}$  is rise time of the instrument.

**B trigger, minimum time between arm and trigger, typical**

320 ps

For trigger after time, this is the time between the end of the time period and the B trigger event.

For trigger after events, this is the time between the last A trigger event and the first B trigger event.

**B trigger after time, time range** 160 ps to 20 seconds

**B trigger after events, event range** 1 to 65,471

**Trigger level ranges**

Source	Range
Any Channel	$\pm 5$ divs from center of screen
Aux In Trigger, typical	$\pm 8 \text{ V}$
Line	Fixed at about 50% of line voltage

This specification applies to logic and pulse thresholds.

**Trigger holdoff range** 0 ns to 20 seconds

## Serial Trigger specifications

**Optional serial bus interface triggering** Please refer to the *Serial Triggering and Analysis Datasheet*, located on the [tek.com](http://tek.com), for information on available serial triggering options and their triggering capabilities.

## Digital acquisition system

**Digital channel maximum sample rate** 6.25 GS/s

**Transition detect (digital peak detect)** Displayed data at sample rates less than 6.25 GS/s (decimated data), that contains multiple transitions between sample points will be displayed with a bright white colored edge.

**Digital-To-Analog trigger skew** 3 ns

**Digital to digital skew** 3 ns from bit 0 of any TekVPI channel to bit 0 of any TekVPI channel.

**Digital skew within a FlexChannel**  
**MSO44, MSO46:** <160 ps within any TekVPI channel  
**MSO44B, MSO46B:** <200 ps within any TekVPI channel

## Digital volt meter (DVM)

**Measurement types** DC, AC<sub>RMS</sub>+DC, AC<sub>RMS</sub>

**Voltage resolution** 4 digits

✓ **Voltage accuracy**

**DC:**  $\pm((1.5\% * |\text{reading} - \text{offset} - \text{position}|) + (0.5\% * |(\text{offset} - \text{position})|)) + (0.1 * \text{Volts/div})$   
 De-rated at 0.100%/°C of |reading - offset - position| above 30 °C  
 Signal  $\pm 5$  divisions from screen center

**AC:** **MSO44, MSO46:**  $\pm 2\%$  (40 Hz to 1 kHz) with no harmonic content outside 40 Hz to 1 kHz range  
**MSO44B, MSO46B:**  $\pm 3\%$  (40 Hz to 1 kHz) with no harmonic content outside 40 Hz to 1 kHz range  
 AC, typical:  $\pm 2\%$  (20 Hz to 10 kHz)  
 For AC measurements, the input channel vertical settings must allow the V<sub>PP</sub> input signal to cover between 4 and 10 divisions and must be fully visible on the screen

## Trigger frequency counter

✓ **Accuracy**  $\pm(1 \text{ count} + \text{time base accuracy} * \text{input frequency})$   
 The signal must be at least 8 mV<sub>pp</sub> or 2 div, whichever is greater.

✓ **Maximum input frequency** 10 Hz to maximum bandwidth of the analog channel  
**MSO44, MSO46:** The signal must be at least 8 mV<sub>pp</sub> or 2 div, whichever is greater.  
**MSO44B, MSO46B:** The signal must be at least 8 mV<sub>pp</sub> or 3 div, whichever is greater.



Resolution 8-digits

## Arbitrary Function Generator system

Function types Arbitrary, sine, square, pulse, ramp, triangle, DC level, Gaussian, Lorentz, exponential rise/fall,  $\sin(x)/x$ , random noise, Haversine, Cardiac

Amplitude range Values are peak-to-peak voltages

Waveform	50 $\Omega$	1 M $\Omega$
Arbitrary	10 mV to 2.5 V	20 mV to 5 V
Sine	10 mV to 2.5 V	20 mV to 5 V
Square	10 mV to 2.5 V	20 mV to 5 V
Pulse	10 mV to 2.5 V	20 mV to 5 V
Ramp	10 mV to 2.5 V	20 mV to 5 V
Triangle	10 mV to 2.5 V	20 mV to 5 V
Gaussian	10 mV to 1.25 V	20 mV to 2.5 V
Lorentz	10 mV to 1.2 V	20 mV to 2.4 V
Exponential Rise	10 mV to 1.25 V	20 mV to 2.5 V
Exponential Fall	10 mV to 1.25 V	20 mV to 2.5 V
Sine(x)/x	10 mV to 1.5 V	20 mV to 3.0 V
Random Noise	10 mV to 2.5 V	20 mV to 5 V
Haversine	10 mV to 1.25 V	20 mV to 2.5 V
Cardiac	10 mV to 2.5 V	20 mV to 5 V

Maximum sample rate 250 MS/s

Arbitrary function record length 128 K Samples

### Sine waveform

Frequency range 0.1 Hz to 50 MHz

Frequency setting resolution 0.1 Hz

Amplitude flatness, typical **MSO44, MSO46:**  $\pm 0.5$  dB at 1 kHz  
**MSO44B, MSO46B:**  $\pm 1.0$  dB at 1 kHz  
 $\pm 1.5$  dB at 1 kHz for  $< 20$  mV<sub>pp</sub> amplitudes

Total harmonic distortion, typical **MSO44, MSO46:** 1% for amplitude  $\geq 200$  mV<sub>pp</sub> into 50  $\Omega$  load  
**MSO44B, MSO46B:** 1.5% for amplitude  $\geq 200$  mV<sub>pp</sub> into 50  $\Omega$  load  
**MSO44, MSO46:** 2.5% for amplitude  $> 50$  mV AND  $< 200$  mV<sub>pp</sub> into 50  $\Omega$  load  
**MSO44B, MSO46B:** 3.5% for amplitude  $> 50$  mV AND  $< 200$  mV<sub>pp</sub> into 50  $\Omega$  load  
 This is for Sine wave only.

**Spurious free dynamic range, typical**      **MSO44, MSO46:** 40 dB ( $V_{pp} \geq 0.1$  V); 30 dB ( $V_{pp} \geq 0.02$  V), 50  $\Omega$  load  
**MSO44B, MSO46B:** 35 dB ( $V_{pp} \geq 0.2$  V), 50  $\Omega$  load

**Square and pulse waveform**

**Frequency range**      0.1 Hz to 25 MHz

**Frequency setting resolution**      0.1 Hz

**Duty cycle range**      10% - 90% or 10 ns minimum pulse, whichever is larger  
 Minimum pulse time applies to both on and off time, so maximum duty cycle will reduce at higher frequencies to maintain 10 ns off time

**Duty cycle resolution**      0.1%

**Minimum pulse width, typical**      10 ns. This is the minimum time for either on or off duration.

**Rise/Fall time, typical**      **MSO44, MSO46:** 5.5 ns, 10% - 90%  
**MSO44B, MSO46B:** 6 ns, 10% - 90%

**Pulse width resolution**      100 ps

**Overshoot, typical**      **MSO44, MSO46:** < 4 % for signal steps greater than 100 mV<sub>pp</sub>  
**MSO44B, MSO46B:** < 6% for signal steps greater than 100 mV<sub>pp</sub>  
 This applies to overshoot of the positive-going transition (+overshoot) and of the negative-going (-overshoot) transition

**Asymmetry, typical**       $\pm 1\% \pm 5$  ns, at 50% duty cycle

**Jitter, typical**      < 60 ps TIE<sub>RMS</sub>,  $\geq 100$  mV<sub>pp</sub> amplitude, 40%-60% duty cycle

**Cardiac maximum frequency**      **MSO44, MSO46:** 1 MHz  
**MSO44B, MSO46B:** 500 kHz

**Ramp and triangle waveform**

**Frequency range**      0.1 Hz to 500 kHz

**Frequency setting resolution**      0.1 Hz

**Variable symmetry**      0% - 100%

**Symmetry resolution**      0.1%

**DC level range**       $\pm 2.5$  V into Hi-Z  
 $\pm 1.25$  V into 50  $\Omega$

**Gaussian pulse, Haversine, and Lorentz pulse**

**Maximum frequency**      5 MHz

**Exponential rise fall maximum frequency**      5 MHz

**Sin(x)/x**

<b>Maximum frequency</b>	2 MHz
<b>Random noise amplitude range</b>	20 mV <sub>pp</sub> to 5 V <sub>pp</sub> into Hi-Z 10 mV <sub>pp</sub> to 2.5 V <sub>pp</sub> into 50 Ω For both isolated noise signal and additive noise signal.
<b>✓ Sine, ramp, square and pulse frequency accuracy</b>	1.3 x 10 <sup>-4</sup> (frequency ≤10 kHz) 5.0 x 10 <sup>-5</sup> (frequency >10 kHz)
<b>Signal amplitude resolution</b>	1 mV (Hi-Z) 500 μV (50 Ω)
<b>✓ Signal amplitude accuracy</b>	±[ (1.5% of peak-to-peak amplitude setting) + (1.5% of absolute DC offset setting) + 1 mV ] (frequency = 1 kHz)
<b>DC offset range</b>	±2.5 V into Hi-Z ±1.25 V into 50 Ω
<b>DC offset resolution</b>	1 mV (Hi-Z) 500 μV (50 Ω)
<b>✓ DC offset accuracy</b>	±[ (1.5% of absolute offset voltage setting) + 1 mV ] Add 3 mV of uncertainty per 10 °C change from 25 °C ambient. Refer <a href="#">DC Offset Accuracy test record</a> on page 42

## Display system

<b>Display type</b>	<b>MSO44, MSO46:</b> Display area - 11.38 inches (289 mm) (H) x 6.51 inches (165 mm) (V), 13.3 inches (338 mm) diagonal, 6-bit RGB color, TFT liquid crystal display (LCD) with capacitive touch  <b>MSO44B, MSO46B:</b> Display area - 11.57 inches (293.76 mm) (H) x 6.5 inches (165.24 mm) (V), 13.3 inches (338 mm) diagonal, 6-bit RGB color, optically-bonded liquid crystal display (LCD) with capacitive touch
<b>Resolution</b>	1,920 horizontal × 1,080 vertical pixels
<b>Luminance, typical</b>	<b>MSO44, MSO46:</b> 400 cd/m <sup>2</sup> , (Minimum: 320 cd/m <sup>2</sup> )  <b>MSO44B, MSO46B:</b> 270 cd/m <sup>2</sup>  Display luminance is specified for a new display set at full brightness.

## Processor system

<b>Host processor</b>	<b>MSO44, MSO46:</b> Texas Instruments AM5728  <b>MSO44B, MSO46B:</b> Intel x6413E at 1.5 GHz (HFM) / 3.0 GHz (Turbo). Elkhart Lake 4-Core.
-----------------------	---

**Operating system** Closed Linux

## Input/Output port specifications

**Ethernet interface** An 8-pin RJ-45 connector that supports 10/100/1000 Mb/s

**Video signal output** A 29-pin HDMI connector

**MSO44, MSO46:** Recommended resolution: 1920 x 1080 @ 60 Hz. Video out may not be hot pluggable. HDMI cable may need to be attached before power up for dual display functions to work depending upon the instrument firmware revision

**MSO44B, MSO46B:** Supported resolution: 1920 x 1080 @ 60 Hz only. Hot plug support.

**USB interface (Host, Device ports)** Front panel USB Host ports: Three USB 2.0 Hi-Speed ports

**MSO44, MSO46:** Rear panel USB Host ports: Two USB 2.0 Hi-Speed ports

**MSO44B, MSO46B:** Rear panel USB Host ports: Two USB 3.1 SuperSpeed ports

Rear panel USB Device port: One USB 2.0 Hi-Speed Device port providing USBTMC support

### Probe compensator signal output voltage and frequency, typical

**Output voltage amplitude:** 2.5 V  $\pm$ 2% (nominally 0-2.5V)

**Output frequency:** 1 kHz  $\pm$ 25%

**Output source impedance** nominally 1k $\Omega$

### Auxiliary output, AUX OUT, Trigger Out, Event, or Reference Clock Out

**Selectable output** Acquisition Trigger Out  
Reference Clock Out  
AFG Trigger Out

**Acquisition Trigger Out** User selectable transition from HIGH to LOW, or LOW to HIGH, indicates the trigger occurred. The signal returns to its previous state after approximately 100 ns

**Acquisition trigger jitter** 380 ps (peak-to-peak)

**Reference Clock Out** Reference clock output tracks the acquisition system and can be referenced from either the internal clock reference or the external clock reference

**AFG Trigger Out** The output frequency is dependent on the frequency of the AFG signal as shown in the following table:

AFG signal frequency	AFT trigger frequency
$\leq$ 4.9 MHz	Signal frequency
> 4.9 MHz to 14.7 MHz	Signal frequency / 3
> 14.7 MHz to 24.5 MHz	Signal frequency / 5
> 24.5 MHz to 34.3 MHz	Signal frequency / 7
> 34.3 MHz to 44.1 MHz	Signal frequency / 9
> 44.1 MHz to 50 MHz	Signal frequency / 11

**AUX OUT Output Voltage**

Characteristic	Limits
Vout (HI)	$\geq 2.5$ V open circuit; $\geq 1.0$ V into a 50 $\Omega$ load to ground
Vout (LO)	$\leq 0.7$ V into a load of $\leq 4$ mA; $\leq 0.25$ V into a 50 $\Omega$ load to ground

**External reference input**

<b>Nominal input frequency</b>	10 MHz
<b>Frequency Variation Tolerance</b>	9.99996 MHz to 10.00004 MHz ( $\pm 4.0 \times 10^{-6}$ )
<b>Sensitivity, typical</b>	$V_{in}$ 1.5 $V_{p-p}$ using a 50 $\Omega$ termination
<b>Maximum input signal</b>	7 $V_{pp}$
<b>Impedance</b>	<b>MSO44, MSO46:</b> 1.2 K Ohms $\pm 20\%$ in parallel with 18 pf $\pm 5$ pf at 10 MHz <b>MSO44B, MSO46B:</b> 800 Ohms $\pm 20\%$ with 18 pf $\pm 20\%$ to ground at 10 MHz

## Data storage specifications

**Nonvolatile memory retention time, typical** No time limit for front panel settings, saved waveforms, setups, product licensing, and calibration constants.

**Real-time clock** A programmable clock providing time in years, months, days, hours, minutes, and seconds.

**MSO44 and MSO46 Nonvolatile memory capacity**

<b>32 GB Primary MMC</b>	Stores the operating system, application software and factory data. No user data
<b>32 GB Secondary MMC</b>	Stores saved setups and waveforms, Ethernet settings, log files, user data and user settings
<b>2 Kbit EEPROM</b>	Memory on the main board that stores the instrument serial number, instrument start up count, total uptime factory data, security option passwords, and user-settable security option passwords
<b>1 Kbit EEPROM</b>	Memory on the main board that stores power management controller factory data
<b>1 KB Flash Memory</b>	Memory on the main board that stores the SODIMM memory configuration data (SPD). Two to four pieces depending on model
<b>32 KB Flash Memory</b>	Memory on the main board that stores microcontroller firmware. Two pieces
<b>64 KB Flash Memory</b>	Memory on the main board that stores microcontroller firmware. Two pieces

**MSO44B and MSO46B Nonvolatile memory capacity**

<b>eMMC 64G</b>	Stores host instrument Linux operating system, application software, and user data including waveforms and measurement results, and instrument settings
	Stores user data and user settings
	Written through the user interface (UI), application software operations, factory operations and programmatic command
	Located on the Processor Board
	User accessible
	To clear, remove and dispose of processor board

	To sanitize, remove and dispose of processor board
<b>NOR Flash 32 MB</b>	Stores host processor bootloader No user data Access method is indirect Written by factory operations Located on the Processor Board Not user accessible Clearing or sanitizing: Not applicable, does not contain user data or settings
<b>2 Kbit EEPROM</b>	Stores factory data, maintenance data No user data Access method is indirect Written by factory operations Located on the Main Board User accessible Clearing or sanitizing: Not applicable, does not contain user data or settings
<b>1 Kbit EEPROM</b>	Stores power management controller factory data, maintenance data No user data Access method is indirect Written by application software operations Located on the Acquisition Board Not user accessible Clearing or sanitizing: Not applicable, does not contain user data or settings
<b>1 Kbit EEPROM</b>	Stores the host processor memory configuration data (SPD) No user data Access method is indirect Written by factory operations Located on the Processor Board Not user accessible Clearing or sanitizing: Not applicable, does not contain user data or settings
<b>1 KB Flash Memory</b>	Two to four pieces depending on model Stores the SODIMM memory configuration data (SPD) No user data Access method is indirect Written by factory operations Located on the Acquisition Board Not user accessible Clearing or sanitizing: Not applicable, does not contain user data or settings
<b>32 KB Flash Memory</b>	Stores power management micro-controller firmware No user data

	<p>Access method is indirect</p> <p>Written by application software operations</p> <p>Internal to the MC9S08 micro-controller on the Main Board</p> <p>Not user accessible</p> <p>Clearing or sanitizing: Not applicable, does not contain user data or settings</p>
<b>32 KB FRAM Memory</b>	<p>Stores host processor power sequencer micro-controller firmware</p> <p>No user data</p> <p>Access method is indirect</p> <p>Written by application software operations</p> <p>Internal to the MSP430 micro-controller on the Processor Board</p> <p>Not user accessible</p> <p>Clearing or sanitizing: Not applicable, does not contain user data or settings</p>
<b>64 KB Flash Memory</b>	<p>Stores analog front end micro-controller firmware</p> <p>No user data</p> <p>Access method is indirect</p> <p>Written by application software operations</p> <p>Internal to the KL14 micro-controller on the Acquisition Board</p> <p>Not user accessible</p> <p>Clearing or sanitizing: Not applicable, does not contain user data or settings</p>
<b>256 KB Flash Memory</b>	<p>Stores front panel micro-controller firmware</p> <p>No user data</p> <p>Access method is indirect</p> <p>Written by application software operations</p> <p>Internal to the TIVA TM4C micro-controller on the Acquisition Board</p> <p>Not user accessible</p> <p>Clearing or sanitizing: Not applicable, does not contain user data or settings</p>
<b>64 MB Flash Memory</b>	<p>Stores the FPGA configuration</p> <p>No user data</p> <p>Access method is indirect</p> <p>Written by application software operations</p> <p>Located on the Acquisition Board</p> <p>Not user accessible</p> <p>Clearing or sanitizing: Not applicable, does not contain user data or settings</p>
<b>64 MB Flash Memory</b>	<p>Stores backup copy of the FPGA configuration</p> <p>No user data</p> <p>Access method is indirect</p> <p>Written by application software operations</p> <p>Located on the Acquisition Board</p> <p>Not user accessible</p>

Clearing or sanitizing: Not applicable, does not contain user data or settings

## Power supply system

### Power

Power consumption	400 Watts maximum
Source voltage	100 - 240 V $\pm$ 10% (50 Hz to 60 Hz)
Source frequency	50 Hz to 60 Hz $\pm$ 10%, at 100 - 240 V $\pm$ 10%
Fuse Rating	12.5 A, 250 V <sub>ac</sub>

## Safety characteristics

Safety certification	<p>US NRTL Listed - UL61010-1 and UL61010-2-030</p> <p>Canadian Certification - CAN/CSA-C22.2 No. 61010.1 and CAN/CSA-C22.2 No 61010.2.030</p> <p>EU Compliance - Low Voltage Directive 2014-35-EU and EN61010-1.</p> <p>International Compliance - IEC 61010-1 and IEC61010-2-030</p>
Pollution degree	Pollution degree 2, indoor, dry location use only
Electrical specification	Measurement CAT II (300V)

## Environmental specifications

### Temperature

Operating	+0 °C to +50 °C (32 °F to 122 °F)
Non-operating	<p><b>MSO44, MSO46:</b> -30 °C to +70 °C (-22 °F to 158 °F)</p> <p><b>MSO44B, MSO46B:</b> -20 °C to +60 °C (-4 °F to 140 °F)</p>

### Humidity

Operating	<p>5% to 90% relative humidity (% RH) at up to +40 °C</p> <p>5% to 50% RH above +40 °C up to +50 °C, noncondensing, and as limited by a maximum wet-bulb temperature of +39 °C</p>
Non-operating	<p>5% to 90% relative humidity (% RH) at up to +40 °C</p> <p>5% to 50% RH above +40 °C up to +50 °C, noncondensing, and as limited by a maximum wet-bulb temperature of +39 °C</p>

### Altitude

Operating	Up to 3,000 meters (9,843 feet)
Non-operating	Up to 12,000 meters (39,370 feet)



<b>Operating random vibration</b>	<b>MSO44B, MSO46B:</b> 0.31 GRMS, 5-500 Hz, 10 minutes per axis, 3 axes (30 minutes total)
<b>Operating mechanical shock</b>	<b>MSO44B, MSO46B:</b> Half-sine mechanical shocks, 40 g peak amplitude, 11 msec duration, 3 drops in each direction of each axis (18 total)

## Mechanical specifications

### Dimensions

<b>Height</b>	11.299 in (286.99 mm) with feet folded in, handle to back
	13.8 in (351 mm) with feet folded in, handle up
<b>Width</b>	15.9 in (405 mm) from handle hub to handle hub
<b>Depth</b>	6.1 in (155 mm) from back of feet to front of knobs, handle up
	10.4 in (265 mm) feet folded in, handle to the back

<b>Weight</b>	<b>MSO44, MSO46:</b> < 16.8 lbs (7.6 kg)
	<b>MSO44B:</b> < 15.96 lbs (7.25 kg)
	<b>MSO46B:</b> < 16.55 lbs (7.52 kg)

<b>Cooling</b>	The clearance requirement for adequate cooling is 2.0 in (50.8 mm) on the right side of the instrument (when viewed from the front) and on the rear of the instrument
----------------	---

<b>Rackmount</b>	Unit fits into rackmount configuration (7U)
------------------	---

<b>MSO44B and MSO46B Audible noise</b>	Audible noise (fan noise) produced by the instrument at ambient temperature (=28°C): = 47 dB
--	--

<b>Kensington lock</b>	Instrument includes a Kensington lock
------------------------	---------------------------------------

## Performance verification procedures

This chapter contains performance verification procedures for the specifications marked with the ✓ symbol. The following equipment, or a suitable equivalent, is required to complete these procedures.

These procedures verify the performance of your instrument. They do not adjust your instrument. If your instrument fails any of the performance verification tests, repeat the failing test, verifying that the test equipment and settings are correct. If the instrument continues to fail a test, contact Tektronix Customer Support for assistance.

These procedures cover all 4 Series MSO instruments. Completion of the performance verification procedure does not update the calibration time and date shown on the **Utility > Calibration** menu.

Print the test records on the following pages and use them to record the performance test results for your oscilloscope. Disregard checks and test records that do not apply to the specific model you are testing. All tests require a 20 minute minimum warm-up period unless otherwise noted.

The following table lists the required equipment. You might need additional cables and adapters, depending on the actual test equipment you use.

Required equipment	Minimum requirements	Example
DC voltage source	3 mV to 4 V, $\pm 0.1$ % accuracy	Fluke 9500B Oscilloscope Calibrator with a 9530 Output Module
Leveled sine wave generator	50 kHz to 2 GHz, $\pm 4$ % amplitude accuracy	
Time mark generator	80 ms period, $\pm 1.0 \times 10^{-6}$ accuracy, rise time <50 ns	
Logic probe	Low capacitance digital probe, 8 channels.	TLP058 probe
BNC-to-0.1 inch pin adapter to connect the logic probe to the signal source.	BNC-to-0.1 inch pin adapter; female BNC to 2x16 .01 inch pin headers.	Tektronix adapter part number 878-1429-00; to connect the Fluke 9500B to the TLP058 probe.
Digital multimeter (DMM)	0.1 % accuracy or better	Tektronix DMM4020
One 50 $\Omega$ terminator	Impedance 50 $\Omega$ ; connectors: female BNC input, male BNC output	Tektronix part number 011-0049-02
One 50 $\Omega$ BNC cable	Male-to-male connectors	Tektronix part number 012-0057-01
Optical mouse	USB, PS2	Tektronix part number 119-7054-00
RF vector signal generator	Maximum bandwidth of instrument	Tektronix TSG4100A

## Test record

### Instrument information, self test record

Model	Serial #	Procedure performed by	Date

Test	Passed	Failed
Self Test		

### Input Impedance test record

Input Impedance				
Performance checks	Vertical scale	Low limit	Test result	High limit
<b>All models</b>				
Channel 1 Input Impedance, 1 M $\Omega$	100 mV/div	990 k $\Omega$		1.01 M $\Omega$
Channel 1 Input Impedance, 50 $\Omega$	10 mV/div	49.5 $\Omega$		50.5 $\Omega$
	100 mV/div	49.5 $\Omega$		50.5 $\Omega$
Channel 2 Input Impedance, 1 M $\Omega$	100 mV/div	990 k $\Omega$		1.01 M $\Omega$
Channel 2 Input Impedance, 50 $\Omega$	10 mV/div	49.5 $\Omega$		50.5 $\Omega$
	100 mV/div	49.5 $\Omega$		50.5 $\Omega$
Channel 3 Input Impedance, 1 M $\Omega$	100 mV/div	990 k $\Omega$		1.01 M $\Omega$
Channel 3 Input Impedance, 50 $\Omega$	10 mV/div	49.5 $\Omega$		50.5 $\Omega$
	100 mV/div	49.5 $\Omega$		50.5 $\Omega$
Channel 4 Input Impedance, 1 M $\Omega$	100 mV/div	990 k $\Omega$		1.01 M $\Omega$
Channel 4, Input Impedance, 50 $\Omega$	10 mV/div	49.5 $\Omega$		50.5 $\Omega$
	100 mV/div	49.5 $\Omega$		50.5 $\Omega$

Input Impedance				
Performance checks	Vertical scale	Low limit	Test result	High limit
<b>6 Channel Models</b>				
Channel 5 Input Impedance, 1 M $\Omega$	100 mV/div	990 k $\Omega$		1.01 M $\Omega$
Channel 5 Input Impedance, 50 $\Omega$	10 mV/div	49.5 $\Omega$		50.5 $\Omega$
	100 mV/div	49.5 $\Omega$		50.5 $\Omega$
Channel 6 Input Impedance, 1 M $\Omega$	100 mV/div	990 k $\Omega$		1.01 M $\Omega$

Table continued...

Input Impedance				
Performance checks	Vertical scale	Low limit	Test result	High limit
<b>6 Channel Models</b>				
Channel 6 Input Impedance, 50 Ω	10 mV/div	49.5 Ω		50.5 Ω
	100 mV/div	49.5 Ω		50.5 Ω

### DC Gain Accuracy test record

DC Gain Accuracy					
Performance checks	Bandwidth	Vertical scale	Low limit	Test result	High limit
<b>All models</b>					
Channel 1 DC Gain Accuracy, 0 V offset, 0 V vertical position, 50 Ω	20 MHz	1 mV/div	-2.5%		2.5%
		2 mV/div	-1%		1%
		5 mV/div	-1%		1%
		10 mV/div	-1%		1%
		20 mV/div	-1%		1%
		50 mV/div	-1%		1%
		100 mV/div	-1%		1%
		200 mV/div	-1%		1%
		500 mV/div	-1%		1%
		1 V/div	-1%		1%
	250 MHz	20 mV/div	-1%		1%
	FULL	20 mV/div	-1%		1%
Channel 1 DC Gain Accuracy, 0 V offset, 0 V vertical position, 1 MΩ	20 MHz	1 mV/div	-2%		2%
		2 mV/div	-1%		1%
		5 mV/div	-1%		1%
		10 mV/div	-1%		1%
		20 mV/div	-1%		1%
		50 mV/div	-1%		1%
		100 mV/div	-1%		1%
		200 mV/div	-1%		1%
		500 mV/div	-1%		1%
		1 V/div	-1%		1%
	250 MHz	20 mV/div	-1%		1%
	FULL	20 mV/div	-1%		1%

Table continued...

DC Gain Accuracy					
Performance checks	Bandwidth	Vertical scale	Low limit	Test result	High limit
<b>All models</b>					
Channel 2 DC Gain Accuracy, 0 V offset, 0 V vertical position, 50 $\Omega$	20 MHz	1 mV/div	-2.5%		2.5%
		2 mV/div	-1%		1%
		5 mV/div	-1%		1%
		10 mV/div	-1%		1%
		20 mV/div	-1%		1%
		50 mV/div	-1%		1%
		100 mV/div	-1%		1%
		200 mV/div	-1%		1%
		500 mV/div	-1%		1%
		1 V/div	-1%		1%
	250 MHz	20 mV/div	-1%		1%
	FULL	20 mV/div	-1%		1%
	Channel 2 DC Gain Accuracy, 0 V offset, 0 V vertical position, 1 M $\Omega$	20 MHz	1 mV/div	-2%	
2 mV/div			-1%		1%
5 mV/div			-1%		1%
10 mV/div			-1%		1%
20 mV/div			-1%		1%
50 mV/div			-1%		1%
100 mV/div			-1%		1%
200 mV/div			-1%		1%
500 mV/div			-1%		1%
1 V/div			-1%		1%
250 MHz		20 mV/div	-1%		1%
FULL		20 mV/div	-1%		1%

Table continued...

DC Gain Accuracy					
Performance checks	Bandwidth	Vertical scale	Low limit	Test result	High limit
<b>All models</b>					
Channel 3 DC Gain Accuracy, 0 V offset, 0 V vertical position, 50 Ω	20 MHz	1 mV/div	-2.5%		2.5%
		2 mV/div	-1%		1%
		5 mV/div	-1%		1%
		10 mV/div	-1%		1%
		20 mV/div	-1%		1%
		50 mV/div	-1%		1%
		100 mV/div	-1%		1%
		200 mV/div	-1%		1%
		500 mV/div	-1%		1%
		1 V/div	-1%		1%
	250 MHz	20 mV/div	-1%		1%
	FULL	20 mV/div	-1%		1%
Channel 3 DC Gain Accuracy, 0 V offset, 0 V vertical position, 1 MΩ	20 MHz	1 mV/div	-2%		2%
		2 mV/div	-1%		1%
		5 mV/div	-1%		1%
		10 mV/div	-1%		1%
		20 mV/div	-1%		1%
		50 mV/div	-1%		1%
		100 mV/div	-1%		1%
		200 mV/div	-1%		1%
		500 mV/div	-1%		1%
		1 V/div	-1%		1%
	250 MHz	20 mV/div	-1%		1%
	FULL	20 mV/div	-1%		1%

Table continued...

DC Gain Accuracy					
Performance checks	Bandwidth	Vertical scale	Low limit	Test result	High limit
<b>All models</b>					
Channel 4 DC Gain Accuracy, 0 V offset, 0 V vertical position, 50 $\Omega$	20 MHz	1 mV/div	-2.5%		2.5%
		2 mV/div	-1%		1%
		5 mV/div	-1%		1%
		10 mV/div	-1%		1%
		20 mV/div	-1%		1%
		50 mV/div	-1%		1%
		100 mV/div	-1%		1%
		200 mV/div	-1%		1%
		500 mV/div	-1%		1%
		1 V/div	-1%		1%
	250 MHz	20 mV/div	-1%		1%
	FULL	20 mV/div	-1%		1%
	Channel 4 DC Gain Accuracy, 0 V offset, 0 V vertical position, 1 M $\Omega$	20 MHz	1 mV/div	-2%	
2 mV/div			-1%		1%
5 mV/div			-1%		1%
10 mV/div			-1%		1%
20 mV/div			-1%		1%
50 mV/div			-1%		1%
100 mV/div			-1%		1%
200 mV/div			-1%		1%
500 mV/div			-1%		1%
1 V/div			-1%		1%
250 MHz		20 mV/div	-1%		1%
FULL		20 mV/div	-1%		1%

DC Gain Accuracy					
Performance checks	Bandwidth	Vertical scale	Low limit	Test result	High limit
<b>6 channel model</b>					
Channel 5 DC Gain Accuracy, 0 V offset, 0 V vertical position, 50 Ω	20 MHz	1 mV/div	-2.5%		2.5%
		2 mV/div	-1%		1%
		5 mV/div	-1%		1%
		10 mV/div	-1%		1%
		20 mV/div	-1%		1%
		50 mV/div	-1%		1%
		100 mV/div	-1%		1%
		200 mV/div	-1%		1%
		500 mV/div	-1%		1%
		1 V/div	-1%		1%
	250 MHz	20 mV/div	-1%		1%
	FULL	20 mV/div	-1%		1%
Channel 5 DC Gain Accuracy, 0 V offset, 0 V vertical position, 1 MΩ	20 MHz	1 mV/div	-2%		2%
		2 mV/div	-1%		1%
		5 mV/div	-1%		1%
		10 mV/div	-1%		1%
		20 mV/div	-1%		1%
		50 mV/div	-1%		1%
		100 mV/div	-1%		1%
		200 mV/div	-1%		1%
		500 mV/div	-1%		1%
		1 V/div	-1%		1%
	250 MHz	20 mV/div	-1%		1%
	FULL	20 mV/div	-1%		1%

Table continued...



DC Gain Accuracy					
Performance checks	Bandwidth	Vertical scale	Low limit	Test result	High limit
<b>6 channel model</b>					
Channel 6 DC Gain Accuracy, 0 V offset, 0 V vertical position, 50 $\Omega$	20 MHz	1 mV/div	-2.5%		2.5%
		2 mV/div	-1%		1%
		5 mV/div	-1%		1%
		10 mV/div	-1%		1%
		20 mV/div	-1%		1%
		50 mV/div	-1%		1%
		100 mV/div	-1%		1%
		200 mV/div	-1%		1%
		500 mV/div	-1%		1%
		1 V/div	-1%		1%
	250 MHz	20 mV/div	-1%		1%
	FULL	20 mV/div	-1%		1%
Channel 6 DC Gain Accuracy, 0 V offset, 0 V vertical position, 1 M $\Omega$	20 MHz	1 mV/div	-2%		2%
		2 mV/div	-1%		1%
		5 mV/div	-1%		1%
		10 mV/div	-1%		1%
		20 mV/div	-1%		1%
		50 mV/div	-1%		1%
		100 mV/div	-1%		1%
		200 mV/div	-1%		1%
		500 mV/div	-1%		1%
		1 V/div	-1%		1%
	250 MHz	20 mV/div	-1%		1%
	FULL	20 mV/div	-1%		1%

## DC Offset Accuracy test record

Use the vertical offset value for both the calibrator output and the oscilloscope offset setting.

Offset Accuracy					
Performance checks	Vertical scale	Vertical offset	Low limit	Test result	High limit
<b>All models</b>					
Channel 1 DC Offset Accuracy, 20 MHz BW, 50 Ω	1 mV/div	900 mV	890.8 mV		909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	5.0 V	4.93 V		5.07 V
	100 mV/div	-5.0 V	-5.07 V		-4.93 V
Channel 1 DC Offset Accuracy, 20 MHz BW, 1 MΩ	1 mV/div	900 mV	890.8 mV		-909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	9.0 V	8.89 V		9.11 V
	100 mV/div	-9.0 V	-9.11 V		-8.89 V
	500 mV/div	9.0 V	8.81 V		9.19 V
	500 mV/div	-9.0 V	-9.19 V		-8.81 V
	1.01 V/div	99.5 V	98.303 V		100.697 V
	1.01 V/div	-99.5 V	-100.697 V		-98.303 V
	5 V/div	99.5 V	97.505 V		101.495 V
	5 V/div	-99.5 V	-101.495 V		-97.505 V
Channel 2 DC Offset Accuracy, 20 MHz BW, 50 Ω	1 mV/div	900 mV	890.8 mV		909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	5.0 V	4.93 V		5.07 V
	100 mV/div	-5.0 V	-5.07 V		-4.93 V
Channel 2 DC Offset Accuracy, 20 MHz BW, 1 MΩ	1 mV/div	900 mV	890.8 mV		-909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	9.0 V	8.89 V		9.11 V
	100 mV/div	-9.0 V	-9.11 V		-8.89 V
	500 mV/div	9.0 V	8.81 V		9.19 V
	500 mV/div	-9.0 V	-9.19 V		-8.81 V
	1.01 V/div	99.5 V	98.303 V		100.697 V
	1.01 V/div	-99.5 V	-100.697 V		-98.303 V
	5 V/div	99.5 V	97.505 V		101.495 V
	5 V/div	-99.5 V	-101.495 V		-97.505 V
Channel 3 DC Offset Accuracy, 20 MHz BW, 50 Ω	1 mV/div	900 mV	890.8 mV		909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	5.0 V	4.93 V		5.07 V
	100 mV/div	-5.0 V	-5.07 V		-4.93 V

Table continued...

Offset Accuracy					
Performance checks	Vertical scale	Vertical offset	Low limit	Test result	High limit
Channel 3 DC Offset Accuracy, 20 MHz BW, 1 M $\Omega$	1 mV/div	900 mV	890.8 mV		-909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	9.0 V	8.89 V		9.11 V
	100 mV/div	-9.0 V	-9.11 V		-8.89 V
	500 mV/div	9.0 V	8.81 V		9.19 V
	500 mV/div	-9.0 V	-9.19 V		-8.81 V
	1.01 V/div	99.5 V	98.303 V		100.697 V
	1.01 V/div	-99.5 V	-100.697 V		-98.303 V
	5 V/div	99.5 V	97.505 V		101.495 V
	5 V/div	-99.5 V	-101.495 V		-97.505 V
Channel 4 DC Offset Accuracy, 20 MHz BW, 50 $\Omega$	1 mV/div	900 mV	890.8 mV		909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	5.0 V	4.93 V		5.07 V
	100 mV/div	-5.0 V	-5.07 V		-4.93 V
Channel 4 DC Offset Accuracy, 20 MHz BW, 1 M $\Omega$	1 mV/div	900 mV	890.8 mV		-909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	9.0 V	8.89 V		9.11 V
	100 mV/div	-9.0 V	-9.11 V		-8.89 V
	500 mV/div	9.0 V	8.81 V		9.19 V
	500 mV/div	-9.0 V	-9.19 V		-8.81 V
	1.01 V/div	99.5 V	98.303 V		100.697 V
	1.01 V/div	-99.5 V	-100.697 V		-98.303 V
	5 V/div	99.5 V	97.505 V		101.495 V
	5 V/div	-99.5 V	-101.495 V		-97.505 V
<b>6 channel model</b>					
Channel 5 DC Offset Accuracy, 20 MHz BW, 50 $\Omega$	1 mV/div	900 mV	890.8 mV		909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	5.0 V	4.93 V		5.07 V
	100 mV/div	-5.0 V	-5.07 V		-4.93 V

Table continued...

Offset Accuracy					
Performance checks	Vertical scale	Vertical offset	Low limit	Test result	High limit
Channel 5 DC Offset Accuracy, 20 MHz BW, 1 MΩ	1 mV/div	900 mV	890.8 mV		-909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	9.0 V	8.89 V		9.11 V
	100 mV/div	-9.0 V	-9.11 V		-8.89 V
	500 mV/div	9.0 V	8.81 V		9.19 V
	500 mV/div	-9.0 V	-9.19 V		-8.81 V
	1.01 V/div	99.5 V	98.303 V		100.697 V
	1.01 V/div	-99.5 V	-100.697 V		-98.303 V
	5 V/div	99.5 V	97.505 V		101.495 V
	5 V/div	-99.5 V	-101.495 V		-97.505 V
Channel 6 DC Offset Accuracy, 20 MHz BW, 50 Ω	1 mV/div	900 mV	890.8 mV		909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	5.0 V	4.93 V		5.07 V
	100 mV/div	-5.0 V	-5.07 V		-4.93 V
Channel 6 DC Offset Accuracy, 20 MHz BW, 1 MΩ	1 mV/div	900 mV	890.8 mV		-909.2 mV
	1 mV/div	-900 mV	-909.2 mV		-890.8 mV
	100 mV/div	9.0 V	8.89 V		9.11 V
	100 mV/div	-9.0 V	-9.11 V		-8.89 V
	500 mV/div	9.0 V	8.81 V		9.19 V
	500 mV/div	-9.0 V	-9.19 V		-8.81 V
	1.01 V/div	99.5 V	98.303 V		100.697 V
	1.01 V/div	-99.5 V	-100.697 V		-98.303 V
	5 V/div	99.5 V	97.505 V		101.495 V
	5 V/div	-99.5 V	-101.495 V		-97.505 V

### Analog Bandwidth test record

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	V <sub>in-pp</sub>	V <sub>bw-pp</sub>	Limit	Test result Gain = V <sub>bw-pp</sub> /V <sub>in-pp</sub>
All 1.5 GHz models							
Table continued...							

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 1	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 1	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 2	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 2	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 3	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 3	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 4		1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 4	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

All 6 channel 1.5 GHz models

Table continued...



Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 5	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 5	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 6	50 $\Omega$	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 6	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

**1 GHz models**

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 1	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 1	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 2	50 $\Omega$	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 2	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 3	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 3	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 4	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 4	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

**1 GHz MSO46**

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 5	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 5	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 6	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 6	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

**500 MHz models**

Table continued...



Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 1	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 1	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 2	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 2	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 3	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 3	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 4		1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 4	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

**500 MHz models (MSO46)**

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 5	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 5	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 6	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 6	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

**350 MHz models**

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 1	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 1	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 2	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 2	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...



Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 3	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 3	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 4	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 4	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

**Six channel models (MSO46)**

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 5	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 5	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 6	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 6	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

**200 MHz**

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 1	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 1	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 2	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 2	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 3	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 3	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 4	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 4	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

**Six channel models (MSO46)**

Table continued...



Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 5	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 5	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

Table continued...

Analog Bandwidth performance checks							
Bandwidth at Channel	Impedance	Vertical scale	Horizontal scale	$V_{in-pp}$	$V_{bw-pp}$	Limit	Test result Gain = $V_{bw-pp}/V_{in-pp}$
Channel 6	50 $\Omega$	1 mV/div	5 ns/div (Full BW)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (Full BW)			$\geq 0.707$	
		5 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		10 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		50 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		100 mV/div	1 ns/div (Full BW)			$\geq 0.707$	
		1 V/div	1 ns/div (Full BW)			$\geq 0.707$	
Channel 6	1 M $\Omega$ , typical	1 mV/div	5 ns/div (500 MHz)			$\geq 0.707$	
		2 mV/div	2.5 ns/div (500 MHz)			$\geq 0.707$	
		5 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		10 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		50 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		100 mV/div	1 ns/div (500 MHz)			$\geq 0.707$	
		1 V/div	1 ns/div (500 MHz)			$\geq 0.707$	

## Random Noise High Res acquisition mode test record

### MS044 and MS046 Random Noise High Res acquisition mode test record

The following test record tables support 4 Series MSO models (MSO44 and MSO46).

Random Noise, Sample acquisition mode: MSO44 and MSO46 1.5 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
MSO44, MSO46 Channel 1	1 mV/div	Full		0.259		0.635
		250 MHz limit				
		20 MHz				
	2 mV/div	Full		0.259		0.635
		250 MHz limit				
		20 MHz				
	5 mV/div	Full		0.271		0.817
		250 MHz limit				
		20 MHz				
	10 mV/div	Full		0.298		0.843
		250 MHz limit				
		20 MHz				
	20 mV/div	Full		0.363		0.92
		250 MHz limit				
		20 MHz				
50 mV/div	Full		0.674		1.582	
	250 MHz limit					
	20 MHz					
100 mV/div	Full		1.609		3.686	
	250 MHz limit					
	20 MHz					
1 V/div	Full		18.561		23.753	
	250 MHz limit					
	20 MHz					
MSO44, MSO46 Channel 2	1 mV/div	Full		0.259		0.635
		250 MHz limit				
		20 MHz				
	2 mV/div	Full		0.259		0.635
		250 MHz limit				
		20 MHz				
	5 mV/div	Full		0.271		0.817
250 MHz limit						
20 MHz						
10 mV/div	Full		0.298		0.843	
	250 MHz limit					

Table continued...

Random Noise, Sample acquisition mode: MSO44 and MSO46 1.5 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	20 mV/div	20 MHz				
		Full		0.363		0.92
		250 MHz limit				
	50 mV/div	20 MHz				
		Full		0.674		1.582
		250 MHz limit				
	100 mV/div	20 MHz				
		Full		1.609		3.686
		250 MHz limit				
	1 V/div	20 MHz				
		Full		18.561		23.753
		250 MHz limit				
<b>MSO44, MSO46 Channel 3</b>	1 mV/div	20 MHz				
		Full		0.259		0.635
		250 MHz limit				
	2 mV/div	20 MHz				
		Full		0.259		0.635
		250 MHz limit				
	5 mV/div	20 MHz				
		Full		0.271		0.817
		250 MHz limit				
	10 mV/div	20 MHz				
		Full		0.298		0.843
		250 MHz limit				
	20 mV/div	20 MHz				
		Full		0.363		0.92
		250 MHz limit				
	50 mV/div	20 MHz				
		Full		0.674		1.582
		250 MHz limit				
	100 mV/div	20 MHz				
		Full		1.609		3.686
		250 MHz limit				
	1 V/div	20 MHz				
		Full		18.561		23.753

Table continued...

Random Noise, Sample acquisition mode: MSO44 and MSO46 1.5 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
		250 MHz limit				
		20 MHz				
<b>MSO44, MSO46 Channel 4</b>	1 mV/div	Full		0.259		0.635
		250 MHz limit				
		20 MHz				
	2 mV/div	Full		0.259		0.635
		250 MHz limit				
		20 MHz				
	5 mV/div	Full		0.271		0.817
		250 MHz limit				
		20 MHz				
	10 mV/div	Full		0.298		0.843
		250 MHz limit				
		20 MHz				
	20 mV/div	Full		0.363		0.92
		250 MHz limit				
		20 MHz				
50 mV/div	Full		0.674		1.582	
	250 MHz limit					
	20 MHz					
100 mV/div	Full		1.609		3.686	
	250 MHz limit					
	20 MHz					
1 V/div	Full		18.561		23.753	
	250 MHz limit					
	20 MHz					
<b>MSO46 Channel 5</b>	1 mV/div	Full		0.259		0.635
		250 MHz limit				
		20 MHz				
	2 mV/div	Full		0.259		0.635
		250 MHz limit				
		20 MHz				
5 mV/div	Full		0.271		0.817	
	250 MHz limit					
	20 MHz					

Table continued...

Random Noise, Sample acquisition mode: MSO44 and MSO46 1.5 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	10 mV/div	Full		0.298		0.843
		250 MHz limit				
		20 MHz				
	20 mV/div	Full		0.363		0.92
		250 MHz limit				
		20 MHz				
	50 mV/div	Full		0.674		1.582
		250 MHz limit				
		20 MHz				
	100 mV/div	Full		1.609		3.686
		250 MHz limit				
		20 MHz				
	1 V/div	Full		18.561		23.753
		250 MHz limit				
		20 MHz				
<b>MSO46 Channel 6</b>	1 mV/div	Full		0.259		0.635
		250 MHz limit				
		20 MHz				
	2 mV/div	Full		0.259		0.635
		250 MHz limit				
		20 MHz				
	5 mV/div	Full		0.271		0.817
		250 MHz limit				
		20 MHz				
	10 mV/div	Full		0.298		0.843
		250 MHz limit				
		20 MHz				
	20 mV/div	Full		0.363		0.92
		250 MHz limit				
		20 MHz				
	50 mV/div	Full		0.674		1.582
		250 MHz limit				
		20 MHz				
	100 mV/div	Full		1.609		3.686
		250 MHz limit				

Table continued...

Random Noise, Sample acquisition mode: MSO44 and MSO46 1.5 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
		20 MHz				
	1 V/div	Full		18.561		23.753
		250 MHz limit				
		20 MHz				

Random Noise, High Res acquisition mode: MSO44 and MSO46 1 GHz models							
Performance Checks			1 M $\Omega$		50 $\Omega$		
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)	
<b>1 GHz models (all models)</b>							
<b>MSO44, MSO46 Channel 1</b>	1 mV/div	Full		0.259		0.336	
		250 MHz limit		0.155		0.161	
		20 MHz		0.096		0.096	
	2 mV/div	Full		0.259		0.363	
		250 MHz limit		0.155		0.161	
		20 MHz		0.096		0.096	
	5 mV/div	Full		0.271		0.394	
		250 MHz limit		0.168		0.174	
		20 MHz		0.096		0.096	
	10 mV/div	Full		0.298		0.434	
		250 MHz limit		0.194		0.206	
		20 MHz		0.103		0.103	
	20 mV/div	Full		0.363		0.551	
		250 MHz limit		0.259		0.298	
		20 MHz		0.129		0.141	
	50 mV/div	Full		0.674		1.038	
		250 MHz limit		0.531		0.596	
		20 MHz		0.233		0.259	
	100 mV/div	Full		1.609		2.102	
		250 MHz limit		1.206		1.349	
		20 MHz		0.596		0.609	
	1 V/div	Full		18.561		16.874	
		250 MHz limit		13.369		11.617	
		20 MHz		7.074		4.906	
	<b>MSO44, MSO46 Channel 2</b>	1 mV/div	Full		0.259		0.336
			250 MHz limit		0.155		0.161

Table continued...

Random Noise, High Res acquisition mode: MSO44 and MSO46 1 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	2 mV/div	20 MHz		0.096		0.096
		Full		0.259		0.363
		250 MHz limit		0.155		0.161
	5 mV/div	20 MHz		0.096		0.096
		Full		0.271		0.394
		250 MHz limit		0.168		0.174
	10 mV/div	20 MHz		0.096		0.096
		Full		0.298		0.434
		250 MHz limit		0.194		0.206
	20 mV/div	20 MHz		0.103		0.103
		Full		0.363		0.551
		250 MHz limit		0.259		0.298
	50 mV/div	20 MHz		0.129		0.141
		Full		0.674		1.038
		250 MHz limit		0.531		0.596
	100 mV/div	20 MHz		0.233		0.259
		Full		1.609		2.102
		250 MHz limit		1.206		1.349
	1 V/div	20 MHz		0.596		0.609
		Full		18.561		16.874
		250 MHz limit		13.369		11.617
<b>MSO44, MSO46 Channel 3</b>	1 mV/div	20 MHz		7.074		4.906
		Full		0.259		0.336
		250 MHz limit		0.155		0.161
	2 mV/div	20 MHz		0.096		0.096
		Full		0.259		0.363
		250 MHz limit		0.155		0.161
	5 mV/div	20 MHz		0.096		0.096
		Full		0.271		0.394
		250 MHz limit		0.168		0.174
	10 mV/div	20 MHz		0.096		0.096
		Full		0.298		0.434
		250 MHz limit		0.194		0.206
	20 mV/div	20 MHz		0.103		0.103
		Full		0.363		0.551

Table continued...



Random Noise, High Res acquisition mode: MSO44 and MSO46 1 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
		250 MHz limit		0.259		0.298
		20 MHz		0.129		0.141
		Full		0.674		1.038
	50 mV/div	250 MHz limit		0.531		0.596
		20 MHz		0.233		0.259
		Full		1.609		2.102
	100 mV/div	250 MHz limit		1.206		1.349
		20 MHz		0.596		0.609
		Full		18.561		16.874
	1 V/div	250 MHz limit		13.369		11.617
		20 MHz		7.074		4.906
		Full		0.259		0.336
<b>MSO44, MSO46 Channel 4</b>	1 mV/div	250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
		Full		0.259		0.363
	2 mV/div	250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
		Full		0.271		0.394
	5 mV/div	250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
		Full		0.298		0.434
	10 mV/div	250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
		Full		0.363		0.551
	20 mV/div	250 MHz limit		0.259		0.298
		20 MHz		0.129		0.141
		Full		0.674		1.038
	50 mV/div	250 MHz limit		0.531		0.596
		20 MHz		0.233		0.259
		Full		1.609		2.102
	100 mV/div	250 MHz limit		1.206		1.349
		20 MHz		0.596		0.609
		Full		18.561		16.874
	1 V/div	250 MHz limit		13.369		11.617
		20 MHz		7.074		4.906
		Full				

Table continued...

Random Noise, High Res acquisition mode: MSO44 and MSO46 1 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
<b>1 GHz models (6 channel model)</b>						
<b>MSO46 Channel 5</b>	1 mV/div	Full		0.259		0.336
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	2 mV/div	Full		0.259		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	5 mV/div	Full		0.271		0.394
		250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
	10 mV/div	Full		0.298		0.434
		250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
	20 mV/div	Full		0.363		0.551
		250 MHz limit		0.259		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.674		1.038
		250 MHz limit		0.531		0.596
		20 MHz		0.233		0.259
	100 mV/div	Full		1.609		2.102
		250 MHz limit		1.206		1.349
		20 MHz		0.596		0.609
	1 V/div	Full		18.561		16.874
		250 MHz limit		13.369		11.617
		20 MHz		7.074		4.906
<b>MSO46 Channel 6</b>	1 mV/div	Full		0.259		0.336
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	2 mV/div	Full		0.259		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	5 mV/div	Full		0.271		0.394
		250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
	10 mV/div	Full		0.298		0.434

Table continued...

Random Noise, High Res acquisition mode: MSO44 and MSO46 1 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
		250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
	20 mV/div	Full		0.363		0.551
		250 MHz limit		0.259		0.298
	50 mV/div	20 MHz		0.129		0.141
		Full		0.674		1.038
		250 MHz limit		0.531		0.596
	100 mV/div	20 MHz		0.233		0.259
		Full		1.609		2.102
		250 MHz limit		1.206		1.349
	1 V/div	20 MHz		0.596		0.609
		Full		18.561		16.874
250 MHz limit			13.369		11.617	
		20 MHz		7.074		4.906

Random Noise, High Res acquisition mode: MSO44 and MSO46 500 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
<b>500 MHz models (all models)</b>						
<b>MSO44, MSO46 Channel 1</b>	1 mV/div	Full		0.259		0.259
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	2 mV/div	Full		0.259		0.259
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	5 mV/div	Full		0.271		0.304
		250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
	10 mV/div	Full		0.298		0.356
		250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
	20 mV/div	Full		0.363		0.466
		250 MHz limit		0.259		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.674		1.038

Table continued...

Random Noise, High Res acquisition mode: MSO44 and MSO46 500 MHz models							
Performance Checks			1 M $\Omega$		50 $\Omega$		
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)	
		250 MHz limit		0.531		0.596	
		20 MHz		0.233		0.259	
		Full		1.609		1.596	
	100 mV/div	250 MHz limit		1.206		1.349	
		20 MHz		0.596		0.609	
		Full		18.561		12.85	
	1 V/div	250 MHz limit		13.369		11.617	
		20 MHz		7.074		4.906	
		Full					
<b>MSO44, MSO46 Channel 2</b>	1 mV/div	Full		0.259		0.259	
		250 MHz limit		0.155		0.161	
		20 MHz		0.096		0.096	
	2 mV/div	Full		0.259		0.259	
		250 MHz limit		0.155		0.161	
		20 MHz		0.096		0.096	
	5 mV/div	Full		0.271		0.304	
		250 MHz limit		0.168		0.174	
		20 MHz		0.096		0.096	
	10 mV/div	Full		0.298		0.356	
		250 MHz limit		0.194		0.206	
		20 MHz		0.103		0.103	
	20 mV/div	Full		0.363		0.466	
		250 MHz limit		0.259		0.298	
		20 MHz		0.129		0.141	
	50 mV/div	Full		0.674		1.038	
		250 MHz limit		0.531		0.596	
		20 MHz		0.233		0.259	
	100 mV/div	Full		1.609		1.596	
		250 MHz limit		1.206		1.349	
		20 MHz		0.596		0.609	
	1 V/div	Full		18.561		12.85	
		250 MHz limit		13.369		11.617	
		20 MHz		7.074		4.906	
	<b>MSO44, MSO46 Channel 3</b>	1 mV/div	Full		0.259		0.259
			250 MHz limit		0.155		0.161
			20 MHz		0.096		0.096

Table continued...

Random Noise, High Res acquisition mode: MSO44 and MSO46 500 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	2 mV/div	Full		0.259		0.259
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	5 mV/div	Full		0.271		0.304
		250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
	10 mV/div	Full		0.298		0.356
		250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
	20 mV/div	Full		0.363		0.466
		250 MHz limit		0.259		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.674		1.038
		250 MHz limit		0.531		0.596
		20 MHz		0.233		0.259
	100 mV/div	Full		1.609		1.596
		250 MHz limit		1.206		1.349
		20 MHz		0.596		0.609
1 V/div	Full		18.561		12.85	
	250 MHz limit		13.369		11.617	
	20 MHz		7.074		4.906	
<b>MSO44, MSO46 Channel 4</b>	1 mV/div	Full		0.259		0.259
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	2 mV/div	Full		0.259		0.259
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	5 mV/div	Full		0.271		0.304
		250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
	10 mV/div	Full		0.298		0.356
		250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
	20 mV/div	Full		0.363		0.466
		250 MHz limit		0.259		0.298

Table continued...

Random Noise, High Res acquisition mode: MSO44 and MSO46 500 MHz models							
Performance Checks			1 M $\Omega$		50 $\Omega$		
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)	
	50 mV/div	20 MHz		0.129		0.141	
		Full		0.674		1.038	
		250 MHz limit		0.531		0.596	
	100 mV/div	20 MHz		0.233		0.259	
		Full		1.609		1.596	
		250 MHz limit		1.206		1.349	
	1 V/div	20 MHz		0.596		0.609	
		Full		18.561		12.85	
		250 MHz limit		13.369		11.617	
		20 MHz		7.074		4.906	
	<b>500 MHz models (6 channel model)</b>						
	<b>MSO46 Channel 5</b>	1 mV/div	Full		0.259		0.259
250 MHz limit				0.155		0.161	
20 MHz				0.096		0.096	
2 mV/div		Full		0.259		0.259	
		250 MHz limit		0.155		0.161	
		20 MHz		0.096		0.096	
5 mV/div		Full		0.271		0.304	
		250 MHz limit		0.168		0.174	
		20 MHz		0.096		0.096	
10 mV/div		Full		0.298		0.356	
		250 MHz limit		0.194		0.206	
		20 MHz		0.103		0.103	
20 mV/div		Full		0.363		0.466	
		250 MHz limit		0.259		0.298	
		20 MHz		0.129		0.141	
50 mV/div		Full		0.674		1.038	
		250 MHz limit		0.531		0.596	
		20 MHz		0.233		0.259	
100 mV/div		Full		1.609		1.596	
		250 MHz limit		1.206		1.349	
		20 MHz		0.596		0.609	
1 V/div		Full		18.561		12.85	
		250 MHz limit		13.369		11.617	
		20 MHz		7.074		4.906	

Table continued...

Random Noise, High Res acquisition mode: MSO44 and MSO46 500 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
MSO46 Channel 6	1 mV/div	Full		0.259		0.259
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	2 mV/div	Full		0.259		0.259
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	5 mV/div	Full		0.271		0.304
		250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
	10 mV/div	Full		0.298		0.356
		250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
	20 mV/div	Full		0.363		0.466
		250 MHz limit		0.259		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.674		1.038
		250 MHz limit		0.531		0.596
		20 MHz		0.233		0.259
	100 mV/div	Full		1.609		1.596
		250 MHz limit		1.206		1.349
		20 MHz		0.596		0.609
1 V/div	Full		18.561		12.85	
	250 MHz limit		13.369		11.617	
	20 MHz		7.074		4.906	

Random Noise, High Res acquisition mode: MSO44 and MSO46 350 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
<b>350 MHz models (all models)</b>						
MSO44, MSO46 Channel 1	1 mV/div	Full		0.181		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	2 mV/div	Full		0.181		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096

Table continued...

Random Noise, High Res acquisition mode: MSO44 and MSO46 350 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	5 mV/div	Full		0.194		0.239
		250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
	10 mV/div	Full		0.206		0.284
		250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
	20 mV/div	Full		0.259		0.349
		250 MHz limit		0.259		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.479		0.139
		250 MHz limit		0.531		0.596
		20 MHz		0.233		0.259
	100 mV/div	Full		1.141		1.349
		250 MHz limit		1.206		1.349
		20 MHz		0.596		0.609
1 V/div	Full		13.239		11.617	
	250 MHz limit		13.369		11.617	
	20 MHz		7.074		4.906	
<b>MSO44, MSO46 Channel 2</b>	1 mV/div	Full		0.181		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	2 mV/div	Full		0.181		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	5 mV/div	Full		0.194		0.239
		250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
	10 mV/div	Full		0.206		0.284
		250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
	20 mV/div	Full		0.259		0.349
		250 MHz limit		0.259		0.298
		20 MHz		0.129		0.141
50 mV/div	Full		0.479		0.139	
	250 MHz limit		0.531		0.596	

Table continued...



Random Noise, High Res acquisition mode: MSO44 and MSO46 350 MHz models							
Performance Checks			1 M $\Omega$		50 $\Omega$		
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)	
	100 mV/div	20 MHz		0.233		0.259	
		Full		1.141		1.349	
		250 MHz limit		1.206		1.349	
	1 V/div	20 MHz		0.596		0.609	
		Full		13.239		11.617	
		250 MHz limit		13.369		11.617	
	<b>MSO44, MSO46 Channel 3</b>	1 mV/div	20 MHz		7.074		4.906
			Full		0.181		0.194
			250 MHz limit		0.155		0.161
2 mV/div		20 MHz		0.096		0.096	
		Full		0.181		0.194	
		250 MHz limit		0.155		0.161	
5 mV/div		20 MHz		0.096		0.096	
		Full		0.194		0.239	
		250 MHz limit		0.168		0.174	
10 mV/div		20 MHz		0.096		0.096	
		Full		0.206		0.284	
		250 MHz limit		0.194		0.206	
20 mV/div		20 MHz		0.103		0.103	
		Full		0.259		0.349	
		250 MHz limit		0.259		0.298	
50 mV/div		20 MHz		0.129		0.141	
		Full		0.479		0.139	
		250 MHz limit		0.531		0.596	
100 mV/div		20 MHz		0.233		0.259	
		Full		1.141		1.349	
		250 MHz limit		1.206		1.349	
1 V/div		20 MHz		0.596		0.609	
		Full		13.239		11.617	
		250 MHz limit		13.369		11.617	
<b>MSO44, MSO46 Channel 4</b>		1 mV/div	20 MHz		7.074		4.906
			Full		0.181		0.194
			250 MHz limit		0.155		0.161
	2 mV/div	20 MHz		0.096		0.096	
		Full		0.181		0.194	
		250 MHz limit		0.155		0.161	

Table continued...

Random Noise, High Res acquisition mode: MSO44 and MSO46 350 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
		Full		0.194		0.239
	5 mV/div	250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
		Full		0.206		0.284
	10 mV/div	250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
		Full		0.259		0.349
	20 mV/div	250 MHz limit		0.259		0.298
		20 MHz		0.129		0.141
		Full		0.479		0.139
	50 mV/div	250 MHz limit		0.531		0.596
		20 MHz		0.233		0.259
		Full		1.141		1.349
	100 mV/div	250 MHz limit		1.206		1.349
		20 MHz		0.596		0.609
		Full		13.239		11.617
	1 V/div	250 MHz limit		13.369		11.617
		20 MHz		7.074		4.906
		<b>350 MHz models (6 channel model)</b>				
MSO46 Channel 5	1 mV/div	Full		0.181		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	2 mV/div	Full		0.181		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.096		0.096
	5 mV/div	Full		0.194		0.239
		250 MHz limit		0.168		0.174
		20 MHz		0.096		0.096
	10 mV/div	Full		0.206		0.284
		250 MHz limit		0.194		0.206
		20 MHz		0.103		0.103
	20 mV/div	Full		0.259		0.349
		250 MHz limit		0.259		0.298
	Table continued...					

Random Noise, High Res acquisition mode: MSO44 and MSO46 350 MHz models							
Performance Checks			1 M $\Omega$		50 $\Omega$		
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)	
	50 mV/div	20 MHz		0.129		0.141	
		Full		0.479		0.139	
		250 MHz limit		0.531		0.596	
	100 mV/div	20 MHz		0.233		0.259	
		Full		1.141		1.349	
		250 MHz limit		1.206		1.349	
	1 V/div	20 MHz		0.596		0.609	
		Full		13.239		11.617	
		250 MHz limit		13.369		11.617	
	MSO46 Channel 6	1 mV/div	20 MHz		7.074		4.906
			Full		0.181		0.194
			250 MHz limit		0.155		0.161
2 mV/div		20 MHz		0.096		0.096	
		Full		0.181		0.194	
		250 MHz limit		0.155		0.161	
5 mV/div		20 MHz		0.096		0.096	
		Full		0.194		0.239	
		250 MHz limit		0.168		0.174	
10 mV/div		20 MHz		0.096		0.096	
		Full		0.206		0.284	
		250 MHz limit		0.194		0.206	
20 mV/div		20 MHz		0.103		0.103	
		Full		0.259		0.349	
		250 MHz limit		0.259		0.298	
50 mV/div		20 MHz		0.129		0.141	
		Full		0.479		0.139	
		250 MHz limit		0.531		0.596	
100 mV/div		20 MHz		0.233		0.259	
		Full		1.141		1.349	
		250 MHz limit		1.206		1.349	
1 V/div		20 MHz		0.596		0.609	
		Full		13.239		11.617	
		250 MHz limit		13.369		11.617	
			20 MHz		7.074		4.906

### MSO44B and MSO46B Random Noise High Res acquisition mode test record

The following test record tables support 4 Series B MSO models (MSO44B and MSO46B).

Random Noise, Sample acquisition mode: MSO44B and MSO46B 1.5 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
MSO44B, MSO46B Channel 1	1 mV/div	Full		0.259		0.674
		250 MHz limit				
		20 MHz				
	2 mV/div	Full		0.271		0.674
		250 MHz limit				
		20 MHz				
	5 mV/div	Full		0.284		0.804
		250 MHz limit				
		20 MHz				
	10 mV/div	Full		0.298		0.804
		250 MHz limit				
		20 MHz				
	20 mV/div	Full		0.389		0.933
		250 MHz limit				
		20 MHz				
	50 mV/div	Full		0.713		1.687
		250 MHz limit				
		20 MHz				
100 mV/div	Full		1.752		3.894	
	250 MHz limit					
	20 MHz					
1 V/div	Full		19.47		27.258	
	250 MHz limit					
	20 MHz					
MSO44B, MSO46B Channel 2	1 mV/div	Full		0.259		0.674
		250 MHz limit				
		20 MHz				
	2 mV/div	Full		0.271		0.674
		250 MHz limit				
		20 MHz				
	5 mV/div	Full		0.284		0.804
		250 MHz limit				
		20 MHz				

Table continued...

Random Noise, Sample acquisition mode: MSO44B and MSO46B 1.5 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	10 mV/div	Full		0.298		0.804
		250 MHz limit				
		20 MHz				
	20 mV/div	Full		0.389		0.933
		250 MHz limit				
		20 MHz				
	50 mV/div	Full		0.713		1.687
		250 MHz limit				
		20 MHz				
	100 mV/div	Full		1.752		3.894
		250 MHz limit				
		20 MHz				
	1 V/div	Full		19.47		27.258
		250 MHz limit				
		20 MHz				
<b>MSO44B, MSO46B Channel 3</b>	1 mV/div	Full		0.259		0.674
		250 MHz limit				
		20 MHz				
	2 mV/div	Full		0.271		0.674
		250 MHz limit				
		20 MHz				
	5 mV/div	Full		0.284		0.804
		250 MHz limit				
		20 MHz				
	10 mV/div	Full		0.298		0.804
		250 MHz limit				
		20 MHz				
	20 mV/div	Full		0.389		0.933
		250 MHz limit				
		20 MHz				
	50 mV/div	Full		0.713		1.687
		250 MHz limit				
		20 MHz				
	100 mV/div	Full		1.752		3.894
		250 MHz limit				

Table continued...

Random Noise, Sample acquisition mode: MSO44B and MSO46B 1.5 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	1 V/div	20 MHz				
		Full		19.47		27.258
		250 MHz limit				
<b>MSO44B, MSO46B Channel 4</b>	1 mV/div	20 MHz				
		Full		0.259		0.674
		250 MHz limit				
	2 mV/div	20 MHz				
		Full		0.271		0.674
		250 MHz limit				
	5 mV/div	20 MHz				
		Full		0.284		0.804
		250 MHz limit				
	10 mV/div	20 MHz				
		Full		0.298		0.804
		250 MHz limit				
	20 mV/div	20 MHz				
		Full		0.389		0.933
		250 MHz limit				
	50 mV/div	20 MHz				
		Full		0.713		1.687
		250 MHz limit				
	100 mV/div	20 MHz				
		Full		1.752		3.894
		250 MHz limit				
	1 V/div	20 MHz				
		Full		19.47		27.258
		250 MHz limit				
<b>MSO46B Channel 5</b>	1 mV/div	20 MHz				
		Full		0.259		0.674
		250 MHz limit				
	2 mV/div	20 MHz				
		Full		0.271		0.674
		250 MHz limit				
	5 mV/div	20 MHz				
		Full		0.284		0.804
		250 MHz limit				

Table continued...

Random Noise, Sample acquisition mode: MSO44B and MSO46B 1.5 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
		250 MHz limit				
		20 MHz				
		Full		0.298		0.804
	10 mV/div	250 MHz limit				
		20 MHz				
		Full		0.389		0.933
	20 mV/div	250 MHz limit				
		20 MHz				
		Full		0.713		1.687
	50 mV/div	250 MHz limit				
		20 MHz				
		Full		1.752		3.894
	100 mV/div	250 MHz limit				
		20 MHz				
		Full		19.47		27.258
1 V/div	250 MHz limit					
	20 MHz					
	Full		0.259		0.674	
<b>MSO46B Channel 6</b>	1 mV/div	250 MHz limit				
		20 MHz				
		Full		0.271		0.674
	2 mV/div	250 MHz limit				
		20 MHz				
		Full		0.284		0.804
	5 mV/div	250 MHz limit				
		20 MHz				
		Full		0.298		0.804
	10 mV/div	250 MHz limit				
		20 MHz				
		Full		0.389		0.933
	20 mV/div	250 MHz limit				
		20 MHz				
		Full		0.713		1.687
	50 mV/div	250 MHz limit				
		20 MHz				
		Full				

Table continued...

Random Noise, Sample acquisition mode: MSO44B and MSO46B 1.5 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	100 mV/div	Full		1.752		3.894
		250 MHz limit				
		20 MHz				
	1 V/div	Full		19.47		27.258
		250 MHz limit				
		20 MHz				

Random Noise, High Res acquisition mode: MSO44B and MSO46B 1 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
<b>1 GHz models (all models)</b>						
<b>MSO44B, MSO46B Channel 1</b>	1 mV/div	Full		0.259		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.271		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.284		0.389
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.298		0.427
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
	20 mV/div	Full		0.389		0.544
		250 MHz limit		0.284		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.713		1.038
		250 MHz limit		0.584		0.596
		20 MHz		0.259		0.259
	100 mV/div	Full		1.752		2.141
		250 MHz limit		1.336		1.349
		20 MHz		0.622		0.609
	1 V/div	Full		19.47		16.874
		250 MHz limit		14.927		11.617
		20 MHz		7.528		4.906

Table continued...



Random Noise, High Res acquisition mode: MSO44B and MSO46B 1 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
MSO44B, MSO46B Channel 2	1 mV/div	Full		0.259		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.271		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.284		0.389
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.298		0.427
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
	20 mV/div	Full		0.389		0.544
		250 MHz limit		0.284		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.713		1.038
		250 MHz limit		0.584		0.596
		20 MHz		0.259		0.259
	100 mV/div	Full		1.752		2.141
		250 MHz limit		1.336		1.349
		20 MHz		0.622		0.609
1 V/div	Full		19.47		16.874	
	250 MHz limit		14.927		11.617	
	20 MHz		7.528		4.906	
MSO44B, MSO46B Channel 3	1 mV/div	Full		0.259		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.271		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.284		0.389
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.298		0.427
250 MHz limit			0.194		0.206	

Table continued...

Random Noise, High Res acquisition mode: MSO44B and MSO46B 1 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	20 mV/div	20 MHz		0.096		0.103
		Full		0.389		0.544
		250 MHz limit		0.284		0.298
	50 mV/div	20 MHz		0.129		0.141
		Full		0.713		1.038
		250 MHz limit		0.584		0.596
	100 mV/div	20 MHz		0.259		0.259
		Full		1.752		2.141
		250 MHz limit		1.336		1.349
	1 V/div	20 MHz		0.622		0.609
		Full		19.47		16.874
		250 MHz limit		14.927		11.617
<b>MSO44B, MSO46B Channel 4</b>	1 mV/div	20 MHz		7.528		4.906
		Full		0.259		0.363
		250 MHz limit		0.155		0.161
	2 mV/div	20 MHz		0.090		0.096
		Full		0.271		0.363
		250 MHz limit		0.155		0.161
	5 mV/div	20 MHz		0.090		0.096
		Full		0.284		0.389
		250 MHz limit		0.168		0.174
	10 mV/div	20 MHz		0.090		0.096
		Full		0.298		0.427
		250 MHz limit		0.194		0.206
	20 mV/div	20 MHz		0.096		0.103
		Full		0.389		0.544
		250 MHz limit		0.284		0.298
	50 mV/div	20 MHz		0.129		0.141
		Full		0.713		1.038
		250 MHz limit		0.584		0.596
	100 mV/div	20 MHz		0.259		0.259
		Full		1.752		2.141
		250 MHz limit		1.336		1.349
	1 V/div	20 MHz		0.622		0.609
		Full		19.47		16.874

Table continued...

Random Noise, High Res acquisition mode: MSO44B and MSO46B 1 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
		250 MHz limit		14.927		11.617
		20 MHz		7.528		4.906
<b>1 GHz models (6 channel model)</b>						
<b>MSO46B Channel 5</b>	1 mV/div	Full		0.259		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.271		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.284		0.389
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.298		0.427
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
	20 mV/div	Full		0.389		0.544
		250 MHz limit		0.284		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.713		1.038
		250 MHz limit		0.584		0.596
		20 MHz		0.259		0.259
	100 mV/div	Full		1.752		2.141
		250 MHz limit		1.336		1.349
		20 MHz		0.622		0.609
	1 V/div	Full		19.47		16.874
		250 MHz limit		14.927		11.617
		20 MHz		7.528		4.906
<b>MSO46B Channel 6</b>	1 mV/div	Full		0.259		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.271		0.363
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.284		0.389
		250 MHz limit		0.168		0.174

Table continued...

Random Noise, High Res acquisition mode: MSO44B and MSO46B 1 GHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	10 mV/div	20 MHz		0.090		0.096
		Full		0.298		0.427
		250 MHz limit		0.194		0.206
	20 mV/div	20 MHz		0.096		0.103
		Full		0.389		0.544
		250 MHz limit		0.284		0.298
	50 mV/div	20 MHz		0.129		0.141
		Full		0.713		1.038
		250 MHz limit		0.584		0.596
	100 mV/div	20 MHz		0.259		0.259
		Full		1.752		2.141
		250 MHz limit		1.336		1.349
	1 V/div	20 MHz		0.622		0.609
		Full		19.47		16.874
		250 MHz limit		14.927		11.617
		20 MHz		7.528		4.906

Random Noise, High Res acquisition mode: MSO44B and MSO46B 500 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
<b>500 MHz models (all models)</b>						
<b>MSO44B, MSO46B Channel 1</b>	1 mV/div	Full		0.259		0.271
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.271		0.271
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.284		0.298
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.298		0.336
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
	20 mV/div	Full		0.389		0.454
		250 MHz limit		0.284		0.298

Table continued...

Random Noise, High Res acquisition mode: MSO44B and MSO46B 500 MHz models							
Performance Checks			1 M $\Omega$		50 $\Omega$		
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)	
	50 mV/div	20 MHz		0.129		0.141	
		Full		0.713		1.012	
		250 MHz limit		0.584		0.596	
	100 mV/div	20 MHz		0.259		0.259	
		Full		1.752		1.674	
		250 MHz limit		1.336		1.349	
	1 V/div	20 MHz		0.622		0.609	
		Full		19.47		12.98	
		250 MHz limit		14.927		11.617	
	<b>MSO44B, MSO46B Channel 2</b>	1 mV/div	20 MHz		7.528		4.906
			Full		0.259		0.271
			250 MHz limit		0.155		0.161
2 mV/div		20 MHz		0.090		0.096	
		Full		0.271		0.271	
		250 MHz limit		0.155		0.161	
5 mV/div		20 MHz		0.090		0.096	
		Full		0.284		0.298	
		250 MHz limit		0.168		0.174	
10 mV/div		20 MHz		0.096		0.103	
		Full		0.298		0.336	
		250 MHz limit		0.194		0.206	
20 mV/div		20 MHz		0.129		0.141	
		Full		0.389		0.454	
		250 MHz limit		0.284		0.298	
50 mV/div		20 MHz		0.259		0.259	
		Full		0.713		1.012	
		250 MHz limit		0.584		0.596	
100 mV/div		20 MHz		0.622		0.609	
		Full		1.752		1.674	
		250 MHz limit		1.336		1.349	
1 V/div		20 MHz		7.528		4.906	
		Full		19.47		12.98	
		250 MHz limit		14.927		11.617	

Table continued...

Random Noise, High Res acquisition mode: MSO44B and MSO46B 500 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
MSO44B, MSO46B Channel 3	1 mV/div	Full		0.259		0.271
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.271		0.271
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.284		0.298
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.298		0.336
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
	20 mV/div	Full		0.389		0.454
		250 MHz limit		0.284		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.713		1.012
		250 MHz limit		0.584		0.596
		20 MHz		0.259		0.259
	100 mV/div	Full		1.752		1.674
		250 MHz limit		1.336		1.349
		20 MHz		0.622		0.609
	1 V/div	Full		19.47		12.98
		250 MHz limit		14.927		11.617
		20 MHz		7.528		4.906
MSO44B, MSO46B Channel 4	1 mV/div	Full		0.259		0.271
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.271		0.271
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.284		0.298
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.298		0.336
		250 MHz limit		0.194		0.206

Table continued...

Random Noise, High Res acquisition mode: MSO44B and MSO46B 500 MHz models							
Performance Checks			1 M $\Omega$		50 $\Omega$		
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)	
		20 MHz		0.096		0.103	
	20 mV/div	Full		0.389		0.454	
		250 MHz limit		0.284		0.298	
		20 MHz		0.129		0.141	
	50 mV/div	Full		0.713		1.012	
		250 MHz limit		0.584		0.596	
		20 MHz		0.259		0.259	
	100 mV/div	Full		1.752		1.674	
		250 MHz limit		1.336		1.349	
		20 MHz		0.622		0.609	
	1 V/div	Full		19.47		12.98	
		250 MHz limit		14.927		11.617	
		20 MHz		7.528		4.906	
<b>500 MHz models (6 channel model)</b>							
<b>MSO46B Channel 5</b>	1 mV/div	Full		0.259		0.271	
		250 MHz limit		0.155		0.161	
		20 MHz		0.090		0.096	
	2 mV/div	Full		0.271		0.271	
		250 MHz limit		0.155		0.161	
		20 MHz		0.090		0.096	
	5 mV/div	Full		0.284		0.298	
		250 MHz limit		0.168		0.174	
		20 MHz		0.090		0.096	
	10 mV/div	Full		0.298		0.336	
		250 MHz limit		0.194		0.206	
		20 MHz		0.096		0.103	
	20 mV/div	Full		0.389		0.454	
		250 MHz limit		0.284		0.298	
		20 MHz		0.129		0.141	
	50 mV/div	Full		0.713		1.012	
		250 MHz limit		0.584		0.596	
		20 MHz		0.259		0.259	
	100 mV/div	Full		1.752		1.674	
		250 MHz limit		1.336		1.349	
		20 MHz		0.622		0.609	
	Table continued...						

Random Noise, High Res acquisition mode: MSO44B and MSO46B 500 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	1 V/div	Full		19.47		12.98
		250 MHz limit		14.927		11.617
		20 MHz		7.528		4.906
<b>MSO46B Channel 6</b>	1 mV/div	Full		0.259		0.271
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.271		0.271
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.284		0.298
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.298		0.336
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
	20 mV/div	Full		0.389		0.454
		250 MHz limit		0.284		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.713		1.012
		250 MHz limit		0.584		0.596
		20 MHz		0.259		0.259
	100 mV/div	Full		1.752		1.674
		250 MHz limit		1.336		1.349
		20 MHz		0.622		0.609
	1 V/div	Full		19.47		12.98
		250 MHz limit		14.927		11.617
		20 MHz		7.528		4.906

Random Noise, High Res acquisition mode: MSO44B and MSO46B 350 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
<b>350 MHz models (all models)</b>						
<b>MSO44B, MSO46B Channel 1</b>	1 mV/div	Full		0.194		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096

Table continued...



Random Noise, High Res acquisition mode: MSO44B and MSO46B 350 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	2 mV/div	Full		0.194		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.206		0.239
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.220		0.284
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
	20 mV/div	Full		0.298		0.349
		250 MHz limit		0.284		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.584		0.739
		250 MHz limit		0.584		0.596
		20 MHz		0.259		0.259
	100 mV/div	Full		1.298		1.349
		250 MHz limit		1.336		1.349
		20 MHz		0.622		0.609
1 V/div	Full		14.927		11.617	
	250 MHz limit		14.927		11.617	
	20 MHz		7.528		4.906	
<b>MSO44B, MSO46B Channel 2</b>	1 mV/div	Full		0.194		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.194		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.206		0.239
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.220		0.284
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
20 mV/div	Full		0.298		0.349	
	250 MHz limit		0.284		0.298	

Table continued...

Random Noise, High Res acquisition mode: MSO44B and MSO46B 350 MHz models							
Performance Checks			1 M $\Omega$		50 $\Omega$		
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)	
	50 mV/div	20 MHz		0.129		0.141	
		Full		0.584		0.739	
		250 MHz limit		0.584		0.596	
	100 mV/div	20 MHz		0.259		0.259	
		Full		1.298		1.349	
		250 MHz limit		1.336		1.349	
	1 V/div	20 MHz		0.622		0.609	
		Full		14.927		11.617	
		250 MHz limit		14.927		11.617	
	<b>MSO44B, MSO46B Channel 3</b>	1 mV/div	20 MHz		7.528		4.906
			Full		0.194		0.194
			250 MHz limit		0.155		0.161
2 mV/div		20 MHz		0.090		0.096	
		Full		0.194		0.194	
		250 MHz limit		0.155		0.161	
5 mV/div		20 MHz		0.090		0.096	
		Full		0.206		0.239	
		250 MHz limit		0.168		0.174	
10 mV/div		20 MHz		0.090		0.096	
		Full		0.220		0.284	
		250 MHz limit		0.194		0.206	
20 mV/div		20 MHz		0.096		0.103	
		Full		0.298		0.349	
		250 MHz limit		0.284		0.298	
50 mV/div		20 MHz		0.129		0.141	
		Full		0.584		0.739	
		250 MHz limit		0.584		0.596	
100 mV/div		20 MHz		0.259		0.259	
		Full		1.298		1.349	
		250 MHz limit		1.336		1.349	
1 V/div		20 MHz		0.622		0.609	
		Full		14.927		11.617	
		250 MHz limit		14.927		11.617	
			20 MHz		7.528		4.906

Table continued...

Random Noise, High Res acquisition mode: MSO44B and MSO46B 350 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
<b>MSO44B, MSO46B Channel 4</b>	1 mV/div	Full		0.194		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.194		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.206		0.239
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.220		0.284
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
	20 mV/div	Full		0.298		0.349
		250 MHz limit		0.284		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.584		0.739
		250 MHz limit		0.584		0.596
		20 MHz		0.259		0.259
	100 mV/div	Full		1.298		1.349
		250 MHz limit		1.336		1.349
		20 MHz		0.622		0.609
	1 V/div	Full		14.927		11.617
		250 MHz limit		14.927		11.617
		20 MHz		7.528		4.906
<b>350 MHz models (6 channel model)</b>						
<b>MSO46B Channel 5</b>	1 mV/div	Full		0.194		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.194		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.206		0.239
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.220		0.284

Table continued...

Random Noise, High Res acquisition mode: MSO44B and MSO46B 350 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
		Full		0.298		0.349
	20 mV/div	250 MHz limit		0.284		0.298
		20 MHz		0.129		0.141
		Full		0.584		0.739
	50 mV/div	250 MHz limit		0.584		0.596
		20 MHz		0.259		0.259
		Full		1.298		1.349
	100 mV/div	250 MHz limit		1.336		1.349
		20 MHz		0.622		0.609
		Full		14.927		11.617
	1 V/div	250 MHz limit		14.927		11.617
		20 MHz		7.528		4.906
		Full				
<b>MSO46B Channel 6</b>	1 mV/div	Full		0.194		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	2 mV/div	Full		0.194		0.194
		250 MHz limit		0.155		0.161
		20 MHz		0.090		0.096
	5 mV/div	Full		0.206		0.239
		250 MHz limit		0.168		0.174
		20 MHz		0.090		0.096
	10 mV/div	Full		0.220		0.284
		250 MHz limit		0.194		0.206
		20 MHz		0.096		0.103
	20 mV/div	Full		0.298		0.349
		250 MHz limit		0.284		0.298
		20 MHz		0.129		0.141
	50 mV/div	Full		0.584		0.739
		250 MHz limit		0.584		0.596
		20 MHz		0.259		0.259
	100 mV/div	Full		1.298		1.349
		250 MHz limit		1.336		1.349
		20 MHz		0.622		0.609

Table continued...

Random Noise, High Res acquisition mode: MSO44B and MSO46B 350 MHz models						
Performance Checks			1 M $\Omega$		50 $\Omega$	
Channel	V/div	Bandwidth	Test result (mV)	High limit (mV)	Test result (mV)	High limit (mV)
	1 V/div	Full		14.927		11.617
		250 MHz limit		14.927		11.617
		20 MHz		7.528		4.906

## Long term sample rate through AFG DC offset accuracy test records

Long Term Sample Rate			
Performance checks	Low limit	Test result	High limit
Long Term Sample Rate	-2 divisions		+2 divisions

Digital Threshold Accuracy, typical						
Performance checks:						
Digital channel	Threshold	V <sub>s-</sub>	V <sub>s+</sub>	Low limit	Test result	High limit
<b>All models</b>						
<b>Channel 1</b>						
D0	0 V			-0.1 V		0.1 V
D1	0 V			-0.1 V		0.1 V
D2	0 V			-0.1 V		0.1 V
D3	0 V			-0.1 V		0.1 V
D4	0 V			-0.1 V		0.1 V
D5	0 V			-0.1 V		0.1 V
D6	0 V			-0.1 V		0.1 V
D7	0 V			-0.1 V		0.1 V
<b>Channel 2</b>						
D0	0 V			-0.1 V		0.1 V
D1	0 V			-0.1 V		0.1 V
D2	0 V			-0.1 V		0.1 V
D3	0 V			-0.1 V		0.1 V
D4	0 V			-0.1 V		0.1 V
D5	0 V			-0.1 V		0.1 V
D6	0 V			-0.1 V		0.1 V
D7	0 V			-0.1 V		0.1 V
<b>Channel 3</b>						
D0	0 V			-0.1 V		0.1 V
D1	0 V			-0.1 V		0.1 V

Table continued...

Digital Threshold Accuracy, typical						
Performance checks:						
Digital channel	Threshold	V <sub>s-</sub>	V <sub>s+</sub>	Low limit	Test result	High limit
D2	0 V			-0.1 V		0.1 V
D3	0 V			-0.1 V		0.1 V
D4	0 V			-0.1 V		0.1 V
D5	0 V			-0.1 V		0.1 V
D6	0 V			-0.1 V		0.1 V
D7	0 V			-0.1 V		0.1 V
<b>Channel 4</b>						
D0	0 V			-0.1 V		0.1 V
D1	0 V			-0.1 V		0.1 V
D2	0 V			-0.1 V		0.1 V
D3	0 V			-0.1 V		0.1 V
D4	0 V			-0.1 V		0.1 V
D5	0 V			-0.1 V		0.1 V
D6	0 V			-0.1 V		0.1 V
D7	0 V			-0.1 V		0.1 V
<b>All 6 channel models</b>						
<b>Channel 5</b>						
D0	0 V			-0.1 V		0.1 V
D1	0 V			-0.1 V		0.1 V
D2	0 V			-0.1 V		0.1 V
D3	0 V			-0.1 V		0.1 V
D4	0 V			-0.1 V		0.1 V
D5	0 V			-0.1 V		0.1 V
D6	0 V			-0.1 V		0.1 V
D7	0 V			-0.1 V		0.1 V
<b>Channel 6</b>						
D0	0 V			-0.1 V		0.1 V
D1	0 V			-0.1 V		0.1 V
D2	0 V			-0.1 V		0.1 V
D3	0 V			-0.1 V		0.1 V
D4	0 V			-0.1 V		0.1 V
D5	0 V			-0.1 V		0.1 V
D6	0 V			-0.1 V		0.1 V
D7	0 V			-0.1 V		0.1 V

AUX Out output voltage levels				
Performance checks	Vout	Low limit	Test result	High limit
Output levels, 1 M $\Omega$ input impedance	Max	$\geq 2.5$ V		n/a
	Min	n/a		$\leq 700$ mV
Output levels, 50 $\Omega$ Input Impedance,	Max	$\geq 1$ V		n/a
	Min	n/a		$\leq 250$ mV

DVM voltage accuracy (DC)					
Channel 1					
Vertical Scale	Input Voltage	Offset Voltage	Low limit	Test result	High limit
1	-5	-5	-5.125		-4.875
0.5	-2	-2	-2.06		-1.94
0.5	-1	-0.5	-1.06		-0.94
0.2	-0.5	-0.5	-0.5225		-0.4775
0.01	0.002	0	0.00097		0.00303
0.2	0.5	0.5	0.4775		0.5225
0.5	1	0.5	0.94		1.06
0.5	2	2	1.94		2.06
1	5	5	4.875		5.125
Channel 2					
Vertical Scale	Input Voltage	Offset Voltage	Low limit	Test result	High limit
1	-5	-5	-5.125		-4.875
0.5	-2	-2	-2.06		-1.94
0.5	-1	-0.5	-1.06		-0.94
0.2	-0.5	-0.5	-0.5225		-0.4775
0.01	0.002	0	0.00097		0.00303
0.2	0.5	0.5	0.4775		0.5225
0.5	1	0.5	0.94		1.06
0.5	2	2	1.94		2.06
1	5	5	4.875		5.125
Channel 3					
Vertical Scale	Input Voltage	Offset Voltage	Low limit	Test result	High limit
1	-5	-5	-5.125		-4.875
0.5	-2	-2	-2.06		-1.94
0.5	-1	-0.5	-1.06		-0.94
0.2	-0.5	-0.5	-0.5225		-0.4775
0.01	0.002	0	0.00097		0.00303
0.2	0.5	0.5	0.4775		0.5225

Table continued...

DVM voltage accuracy (DC)					
0.5	1	0.5	0.94		1.06
0.5	2	2	1.94		2.06
1	5	5	4.875		5.125
Channel 4					
Vertical Scale	Input Voltage	Offset Voltage	Low limit	Test result	High limit
1	-5	-5	-5.125		-4.875
0.5	-2	-2	-2.06		-1.94
0.5	-1	-0.5	-1.06		-0.94
0.2	-0.5	-0.5	-0.5225		-0.4775
0.01	0.002	0	0.00097		0.00303
0.2	0.5	0.5	0.4775		0.5225
0.5	1	0.5	0.94		1.06
0.5	2	2	1.94		2.06
1	5	5	4.875		5.125

DVM voltage accuracy (DC)					
6 channel model					
Channel 5					
Vertical Scale	Input Voltage	Offset Voltage	Low limit	Test result	High limit
1	-5	-5	-5.125		-4.875
0.5	-2	-2	-2.06		-1.94
0.5	-1	-0.5	-1.06		-0.94
0.2	-0.5	-0.5	-0.5225		-0.4775
0.01	0.002	0	0.00097		0.00303
0.2	0.5	0.5	0.4775		0.5225
0.5	1	0.5	0.94		1.06
0.5	2	2	1.94		2.06
1	5	5	4.875		5.125
Channel 6					
Vertical Scale	Input Voltage	Offset Voltage	Low limit	Test result	High limit
1	-5	-5	-5.125		-4.875
0.5	-2	-2	-2.06		-1.94
0.5	-1	-0.5	-1.06		-0.94
0.2	-0.5	-0.5	-0.5225		-0.4775
0.01	0.002	0	0.00097		0.00303
0.2	0.5	0.5	0.4775		0.5225
0.5	1	0.5	0.94		1.06
0.5	2	2	1.94		2.06

Table continued...



DVM voltage accuracy (DC)				
1	5	5	4.875	5.125

DVM voltage accuracy (AC)				
All models				
Channel 1				
Vertical Scale	Input Signal	Low limit	Test result	High limit
5 mV	20 mV <sub>pp</sub> at 1 kHz	9.800 mV		10.200 mV
10 mV	50 mV <sub>pp</sub> at 1 kHz	24.5 mV		25.500 mV
100 mV	0.5 V <sub>pp</sub> at 1 kHz	245.000 mV		255.000 mV
200 mV	1 V <sub>pp</sub> at 1 kHz	490.000 mV		510.000 mV
1 V	5 V <sub>pp</sub> at 1 kHz	2450.0 mV		2550.0 mV
Channel 2				
Vertical Scale	Input Signal	Low limit	Test result	High limit
5 mV	20 mV <sub>pp</sub> at 1 kHz	9.800 mV		10.200 mV
10 mV	50 mV <sub>pp</sub> at 1 kHz	24.5 mV		25.500 mV
100 mV	0.5 V <sub>pp</sub> at 1 kHz	245.000 mV		255.000 mV
200 mV	1 V <sub>pp</sub> at 1 kHz	490.000 mV		510.000 mV
1 V	5 V <sub>pp</sub> at 1 kHz	2450.0 mV		2550.0 mV
Channel 3				
Vertical Scale	Input Signal	Low limit	Test result	High limit
5 mV	20 mV <sub>pp</sub> at 1 kHz	9.800 mV		10.200 mV
10 mV	50 mV <sub>pp</sub> at 1 kHz	24.5 mV		25.500 mV
100 mV	0.5 V <sub>pp</sub> at 1 kHz	245.000 mV		255.000 mV
200 mV	1 V <sub>pp</sub> at 1 kHz	490.000 mV		510.000 mV
1 V	5 V <sub>pp</sub> at 1 kHz	2450.0 mV		2550.0 mV
Channel 4				
Vertical Scale	Input Signal	Low limit	Test result	High limit
5 mV	20 mV <sub>pp</sub> at 1 kHz	9.800 mV		10.200 mV
10 mV	50 mV <sub>pp</sub> at 1 kHz	24.5 mV		25.500 mV
100 mV	0.5 V <sub>pp</sub> at 1 kHz	245.000 mV		255.000 mV
200 mV	1 V <sub>pp</sub> at 1 kHz	490.000 mV		510.000 mV
1 V	5 V <sub>pp</sub> at 1 kHz	2450.0 mV		2550.0 mV
6 channel model				
Channel 5				
Vertical Scale	Input Signal	Low limit	Test result	High limit

Table continued...

<b>DVM voltage accuracy (AC)</b>				
5 mV	20 mV <sub>pp</sub> at 1 kHz	9.800 mV		10.200 mV
10 mV	50 mV <sub>pp</sub> at 1 kHz	24.5 mV		25.500 mV
100 mV	0.5 V <sub>pp</sub> at 1 kHz	245.000 mV		255.000 mV
200 mV	1 V <sub>pp</sub> at 1 kHz	490.000 mV		510.000 mV
1 V	5 V <sub>pp</sub> at 1 kHz	2450.0 mV		2550.0 mV
<b>Channel 6</b>				
Vertical Scale	Input Signal	Low limit	Test result	High limit
5 mV	20 mV <sub>pp</sub> at 1 kHz	9.800 mV		10.200 mV
10 mV	50 mV <sub>pp</sub> at 1 kHz	24.5 mV		25.500 mV
100 mV	0.5 V <sub>pp</sub> at 1 kHz	245.000 mV		255.000 mV
200 mV	1 V <sub>pp</sub> at 1 kHz	490.000 mV		510.000 mV
1 V	5 V <sub>pp</sub> at 1 kHz	2450.0 mV		2550.0 mV

<b>Trigger frequency accuracy and trigger frequency counter maximum input frequency</b>				
<b>All models</b>				
<b>Channel 1</b>	Hz	Low limit	Test result	High limit
	100 Hz	99.99974 Hz		100.00026 Hz
	1 kHz	999.9974 Hz		1.0000026 KHz
	10 kHz	9.999974 KHz		10.000026 kHz
	100 kHz	99.99974 kHz		100.00026 kHz
	1 MHz	999.9974 kHz		1.0000026 MHz
	10 MHz	9.999974 MHz		10.000026 MHz
	100 MHz	99.99974 MHz		100.00026 MHz
	1 GHz (1 GHz models only)	999.9974 MHz		1.0000026 GHz
	1.5 GHz (1.5 GHz models only)	1.499994 GHz		1.5000051 GHz

Table continued...

Trigger frequency accuracy and trigger frequency counter maximum input frequency				
<b>Channel 2</b>	Hz	Low limit	Test result	High limit
	100 Hz	99.99974 Hz		100.00026 Hz
	1 kHz	999.9974 Hz		1.0000026 KHz
	10 kHz	9.999974 KHz		10.000026 kHz
	100 kHz	99.99974 kHz		100.00026 kHz
	1 MHz	999.9974 kHz		1.0000026 MHz
	10 MHz	9.999974 MHz		10.000026 MHz
	100 MHz	99.99974 MHz		100.00026 MHz
	1 GHz (1 GHz models only)	999.9974 MHz		1.0000026 GHz
	1.5 GHz (1.5 GHz models only)	1.499994 GHz		1.5000051 GHz
<b>Channel 3</b>	Hz	Low limit	Test result	High limit
	100 Hz	99.99974 Hz		100.00026 Hz
	1 kHz	999.9974 Hz		1.0000026 KHz
	10 kHz	9.999974 KHz		10.000026 kHz
	100 kHz	99.99974 kHz		100.00026 kHz
	1 MHz	999.9974 kHz		1.0000026 MHz
	10 MHz	9.999974 MHz		10.000026 MHz
	100 MHz	99.99974 MHz		100.00026 MHz
	1 GHz (1 GHz models only)	999.9974 MHz		1.0000026 GHz
	1.5 GHz (1.5 GHz models only)	1.499994 GHz		1.5000051 GHz
<b>Channel 4</b>	Hz	Low limit	Test result	High limit
	100 Hz	99.99974 Hz		100.00026 Hz
	1 kHz	999.9974 Hz		1.0000026 KHz
	10 kHz	9.999974 KHz		10.000026 kHz
	100 kHz	99.99974 kHz		100.00026 kHz
	1 MHz	999.9974 kHz		1.0000026 MHz
	10 MHz	9.999974 MHz		10.000026 MHz
	100 MHz	99.99974 MHz		100.00026 MHz
	1 GHz (1 GHz models only)	999.9974 MHz		1.0000026 GHz
	1.5 GHz (1.5 GHz models only)	1.499994 GHz		1.5000051 GHz

Trigger frequency accuracy and trigger frequency counter maximum input frequency
--

<b>6 channel model</b>
------------------------

Table continued...
--------------------

Trigger frequency accuracy and trigger frequency counter maximum input frequency				
<b>Channel 5</b>	Hz	Low limit	Test result	High limit
	100 Hz	99.99974 Hz		100.00026 Hz
	1 kHz	999.9974 Hz		1.0000026 KHz
	10 kHz	9.999974 KHz		10.000026 kHz
	100 kHz	99.99974 kHz		100.00026 kHz
	1 MHz	999.9974 kHz		1.0000026 MHz
	10 MHz	9.999974 MHz		10.000026 MHz
	100 MHz	99.99974 MHz		100.00026 MHz
	1 GHz (1 GHz models only)	999.9974 MHz		1.0000026 GHz
	1.5 GHz (1.5 GHz models only)	1.499994 GHz		1.5000051 GHz
<b>Channel 6</b>	Hz	Low limit	Test result	High limit
	100 Hz	99.99974 Hz		100.00026 Hz
	1 kHz	999.9974 Hz		1.0000026 KHz
	10 kHz	9.999974 KHz		10.000026 kHz
	100 kHz	99.99974 kHz		100.00026 kHz
	1 MHz	999.9974 kHz		1.0000026 MHz
	10 MHz	9.999974 MHz		10.000026 MHz
	100 MHz	99.99974 MHz		100.00026 MHz
	1 GHz (1 GHz models only)	999.9974 MHz		1.0000026 GHz
	1.5 GHz (1.5 GHz models only)	1.499994 GHz		1.5000051 GHz

AFG sine and ramp frequency accuracy				
Performance checks				
	Waveform type	Minimum	Test result	Maximum
	Sine	0.999950 MHz		1.000050 MHz
	Ramp	499.975 kHz		500.025 kHz

AFG square and pulse frequency accuracy				
Performance checks				
	Waveform type	Minimum	Test result	Maximum
	Sine	0.999950 MHz		1.000050 MHz
	Pulse	0.999950 MHz		1.000050 MHz

AFG signal amplitude accuracy				
Performance checks				
	Amplitude	Minimum	Test result	Maximum
	30.0 mV <sub>PP</sub>	28.55 mV <sub>PP</sub>		31.45 mV <sub>PP</sub>
	300.0 mV <sub>PP</sub>	294.5 mV <sub>PP</sub>		305.5 mV <sub>PP</sub>
	800.0 mV <sub>PP</sub>	787.0 mV <sub>PP</sub>		813.0 mV <sub>PP</sub>
	1.500 V <sub>PP</sub>	1.4765 V <sub>PP</sub>		1.5235 V <sub>PP</sub>
	2.000 V <sub>PP</sub>	1.9690 V <sub>PP</sub>		2.0310 V <sub>PP</sub>
	2.500 V <sub>PP</sub>	2.4615 V <sub>PP</sub>		2.5385 V <sub>PP</sub>

AFG DC offset accuracy				
Performance checks				
	Offset	Minimum	Test result	Maximum
	1.25 V	1.23025 Vdc		1.26975 Vdc
	0 V	-0.001 Vdc		+0.001 Vdc
	-1.25 V	-1.26975		-1.23025 Vdc

## Performance tests

This section contains a collection of manual procedures for checking that the instrument performs as warranted. They check all the characteristics that are designated as checked in *Specifications*. (The characteristics that are checked appear with a ✓ in *Specifications*).

## Prerequisites

The tests in this section comprise an extensive, valid confirmation of performance and functionality when the following requirements are met:

- The instrument must be in its normal operating configuration (no covers removed).
- You must have performed and passed the procedures under *Self Test*. (See [Self test](#) on page 167.)
- A signal-path compensation must have been done within the recommended calibration interval and at a temperature within  $\pm 5$  °C ( $\pm 9$  °F) of the present operating temperature. (If the temperature was within the limits just stated at the time you did the prerequisite *Self Test*, consider this prerequisite met). A signal-path compensation must have been done at an ambient humidity within 25% of the current ambient humidity and after having been at that humidity for at least 4 hours.
- The instrument must have been last adjusted at an ambient temperature between +18 °C and +28 °C (+64 °F and +82 °F), must have been operating for a warm-up period of at least 20 minutes, and must be operating at an ambient temperature as listed in the specifications. The warm-up requirement is usually met in the course of meeting the *Self Test* prerequisites listed above.
- The instrument must be powered from a source maintaining voltage and frequency within the limits described in the *Specifications* section.
- The instrument must be in an environment with temperature, altitude, humidity, and vibration within the operating limits described in the *Specifications* section.

## Self test

This procedure verifies that the instrument passes the internal diagnostics and performs signal path compensation. No test equipment or hookups are required.

Equipment required	Prerequisites
None	Power on the instrument and allow a 20 minute warm-up period before performing this procedure.

1. Run the System Diagnostics (may take a few minutes).
  - a. Disconnect all probes and/or cables from the oscilloscope inputs.
  - b. Tap **Utility > Self Test**. This displays the **Self Test** configuration menu.
  - c. Tap the **Run Self Test** button.
  - d. The internal diagnostics perform an exhaustive verification of proper instrument function. This verification may take several minutes. When the verification is finished, the status of each self test is shown in the menu.
  - e. Verify that the status of all tests is passed.
  - f. Tap anywhere outside the menu to exit the menu.
2. Run the signal-path compensation routine (may take 5 to 15 minutes per channel).
  - a. Tap **Utility > Calibration**. This displays the **Calibration** configuration menu.
  - b. Tap the **Run SPC** button to start the routine.
  - c. Signal-path compensation may take 5 to 15 minutes to run per channel.
  - d. Verify that the **SPC Status** is **Passed**.
3. Return to regular service: Tap anywhere outside the menu to exit the **Calibration** menu.

The self test procedures are completed. If any of the above tests failed, run the tests again. If there are still failures, contact Tektronix Customer Support.



**Note:** You cannot run the remaining performance tests until the self tests pass and the SPC has successfully run.

## Check input impedance

This test checks the input impedance on all channels.


1. Connect the output of the oscilloscope calibrator (for example, Fluke 9500) to the oscilloscope channel 1 input, as shown in the following illustration.



**WARNING:** Be sure to set the generator to Off or 0 volts before connecting, disconnecting, and/or moving the test hookup during the performance of this procedure. The generator is capable of providing dangerous voltages.



**Note:** Impedance measuring equipment that produces a voltage across the channel that exceeds the measurement range of the instrument may report erroneous impedance results. A measurement voltage exceeds the measurement range of the instrument when the resulting trace is not visible on the graticule.

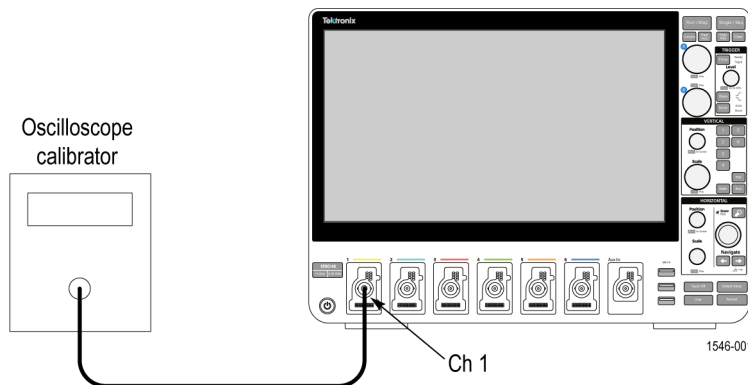


2. Set the calibrator to measure 1 M $\Omega$  impedance.
3. Tap **File > Default Setup**.
4. Test 1 M $\Omega$  input impedance.
  - a. Tap the channel 1 button on the Settings bar.
  - b. Double tap the **Ch 1** badge to open its menu.
  - c. Set **Termination** to 1 M $\Omega$ .
  - d. Set the **Vertical Scale** to the value to test in the test record (first value is 10 mV/div).
5. Use the calibrator to measure the input impedance of the oscilloscope and enter the value in the test record.
6. Repeat steps 4.d on page 119 and 5 on page 119 for all vertical scale settings in the test record for the channel.
7. Test 50  $\Omega$  input impedance as follows:
  - a. Set the calibrator impedance to measure 50  $\Omega$  impedance.
  - b. Double-tap the **Ch 1** badge and set **Termination** to 50  $\Omega$ .
  - c. Repeat steps 4.d on page 119 through 6 on page 119 for all vertical scale settings in the test record for the channel.
8. Repeat the procedures for all remaining channels.
  - a. Turn the calibrator output Off.
  - b. Move the calibrator connection to the next channel to test.
  - c. Double-tap the channel badge of the channel that you have finished testing and set **Display** to **Off**.
  - d. Tap the channel button on the Settings bar of the next channel to test.
  - e. Starting from step 2 on page 119, repeat the procedures until all channels have been tested.

## Check DC gain accuracy

This test checks the DC gain accuracy

1. Connect the oscilloscope to a calibrated DC voltage source. If you are using the Fluke 9500 calibrator, connect the calibrator head to the oscilloscope channel to test.

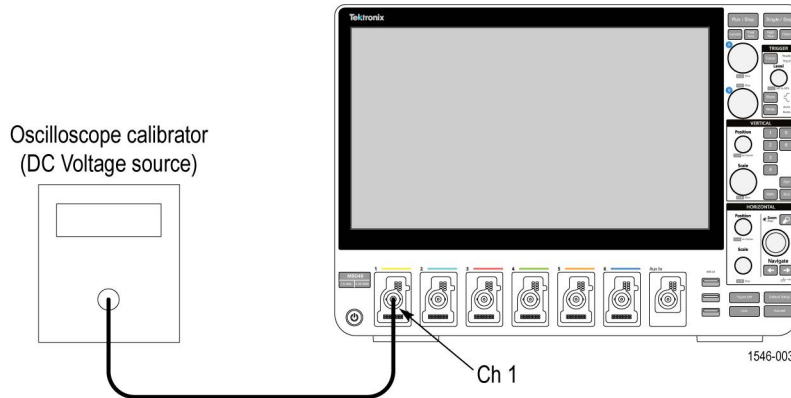

**WARNING:** Set the generator output to Off or 0 volts before connecting, disconnecting, and/or moving the test hookup during the performance of this procedure. The generator is capable of providing dangerous voltages.

2. Tap **File > Default Setup**.
3. Double-tap the **Acquisition** badge and set **Acquisition Mode** to **Average**.
4. Set the **Number of Waveforms** to **16**.
5. Tap outside the menu to close the menu.
6. Double-tap the **Trigger** badge and set the trigger **Source** to **AC line**.
7. Tap outside the menu to close it.
8. Add the **Mean** measurement to the Results bar:
  - a. Tap the **Add New... Measure** button to open the **Add Measurements** menu.
  - b. Set the **Source** to **Ch 1**.
  - c. In the **Amplitude Measurements** panel, double-tap the **Mean** button to add the Mean measurement badge to the Results bar.
9. Tap outside the menu to close it.
10. Double-tap the **Mean** results badge.
11. Tap **Show Statistics in Badge**.
12. Tap **FILTER/LIMIT RESULTS** to open the panel.
13. Tap **Limit Measurement Population** to toggle it to **On**.
14. Tap outside the menu to close it.
15. Tap the channel button of the channel to test, to add the channel badge to the Settings bar.
16. Double tap the channel to test badge to open its menu and set the channel settings:
  - a. Set **Vertical Scale** to **1 mV/div**.
  - b. Set **Termination** to **50 Ω**.
  - c. Tap **Bandwidth Limit** and set to **20 MHz**.
  - d. Tap outside the menu to close it.
17. Record the negative-measured and positive-measured mean readings in the *Expected gain worksheet* as follows:
  - a. On the calibrator, set the DC Voltage Source to the  $V_{\text{negative}}$  value as listed in the 1 mV row of the worksheet.
  - b. Double-tap the **Acquisition** badge and tap **Clear** to reset the measurement statistics.



- c. Enter the **Mean** reading in the worksheet as  $V_{\text{negative-measured}}$ .
- d. On the calibrator, set the DC Voltage Source to  $V_{\text{positive}}$  value as listed in the 1 mV row of the worksheet.
- e. Double-tap the **Acquisition** badge (if not open) and tap **Clear**.
- f. Enter the **Mean** reading in the worksheet as  $V_{\text{positive-measured}}$ .

**Table 1: Expected gain worksheet**

Oscilloscope vertical scale setting	$V_{\text{diffExpected}}$	$V_{\text{negative}}$	$V_{\text{positive}}$	$V_{\text{negative-measured}}$	$V_{\text{positive-measured}}$	$V_{\text{diff}}$	Test result (Gain accuracy)
1 mV/div	7 mV	-3.5 mV	+3.5 mV				
2 mV/div	14 mV	-7 mV	+7 mV				
5 mV/div	35 mV	-17.5 mV	+17.5 mV				
10 mV/div	70 mV	-35 mV	+35 mV				
20 mV/div	140 mV	-70 mV	+70 mV				
50 mV/div	350 mV	-175 mV	+175 mV				
100 mV/div	700 mV	-350 mV	+350 mV				
200 mV/div	1400 mV	-700 mV	+700 mV				
500 mV/div	3500 mV	-1750 mV	+1750 mV				
1.0 V/div	7000 mV	-3500 mV	+3500 mV				
20 mV/div at 250 MHz	140 mV	-70 mV	+70 mV				
20 mV/div at Full BW	140 mV	-70 mV	+ 70 mV				


18. Calculate Gain Accuracy as follows:
  - a. Calculate  $V_{\text{diff}}$  as follows:
 
$$V_{\text{diff}} = | V_{\text{negative-measured}} - V_{\text{positive-measured}} |$$
  - b. Enter  $V_{\text{diff}}$  in the worksheet.
  - c. Calculate *Gain Accuracy* as follows:
 
$$\text{Gain Accuracy} = ((V_{\text{diff}} - V_{\text{diffExpected}}) / V_{\text{diffExpected}}) \times 100\%$$
  - d. Enter the *Gain Accuracy* value in the worksheet and in the test record.
19. Repeat steps 16 on page 120 through 18 on page 121 for all vertical scale settings in the work sheet and the test record.
20. Repeat tests at 1 M $\Omega$  impedance as follows:
  - a. Set the calibrator to 0 volts and 1 M $\Omega$  output impedance.
  - b. Double-tap the badge of the channel being tested.
  - c. Set the **Termination** to 1 M $\Omega$

- d. Repeat steps 16 on page 120 through 19 on page 121 for all vertical scale settings in the test record.
21. Repeat the procedure for all remaining channels:
  - a. Set the calibrator to 0 volts and 50  $\Omega$  output impedance.
  - b. Move the calibrator output to the next channel input to be tested.
  - c. Double-tap the channel badge of the channel that you have finished testing and set **Display** to **Off**.
  - d. Double-tap the **Mean** measurement badge.
  - e. Tap the **Configure** panel.
  - f. Tap the **Source 1** field and select the next channel to test.
  - g. Starting from step 16 on page 120, set the values from the test record for the channel under test, and repeat the above steps until all channels have been tested.
22. Touch outside a menu to close the menu.

## Check DC offset accuracy

This test checks the offset accuracy at 50  $\Omega$  and 1 M $\Omega$  input impedance.

1. Connect the oscilloscope to a calibrated DC voltage source. If you are using the Fluke 9500B calibrator as the DC voltage source, connect the calibrator head to the oscilloscope channel 1.

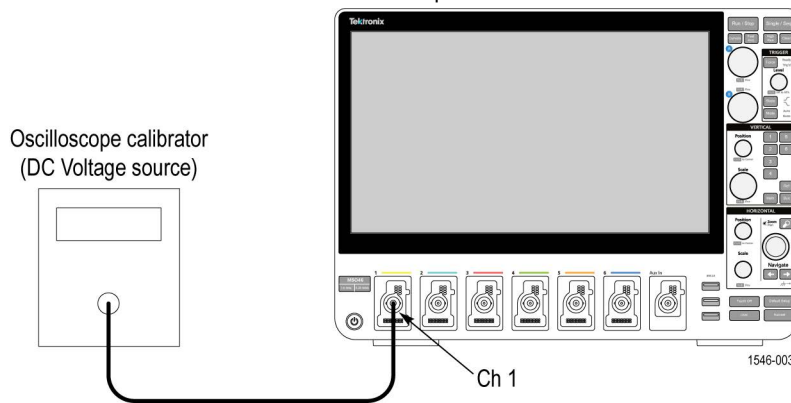

**WARNING:** Set the generator output to Off or 0 volts before connecting, disconnecting, or moving the test hookup during the performance of this procedure. The generator is capable of providing dangerous voltages.


2. Tap **File > Default Setup**.
3. Double-tap the **Acquisition** badge and set **Acquisition Mode** to **Average**.
4. Set the **Number of Waveforms** to 16.
5. Tap outside the menu to close the menu.
6. Double-tap the **Trigger** badge and set the trigger **Source** to **AC line**.
7. Add the **Mean** measurement to the Results bar:
  - a. Tap the **Add New... Measure** button to open the **Add Measurements** menu.
  - b. Set the **Source** to **Ch 1**.
  - c. In the **Amplitude Measurements** panel, double-tap the **Mean** button to add the Mean measurement badge to the Results bar.
8. Tap outside the menu to close it.
9. Double-tap the **Mean** results badge.
10. Tap **Show Statistics in Badge**.
11. Tap **FILTER/LIMIT RESULTS** to open the panel.
12. Tap **Limit Measurement Population** to toggle it to **On**.

13. Tap outside the menu to close it.
14. Tap the channel button on the Settings bar to add the channel under test to the Settings bar.
15. Double-tap the channel under test badge to open its configuration menu and change the vertical settings:
  - a. Set **Vertical Scale** to **1 mV/div**.
  - b. Set **Offset** to **900 mV**.
  - c. Set **Position** to 0 by tapping **Set to 0**.
  - d. Set **Termination** to **50  $\Omega$** .
  - e. Tap **Bandwidth Limit** and set to **20 MHz**.
  - f. Tap outside the menu to close it.
16. Set the calibrator output to **+900 mV**, as shown in the test record, and turn the calibrator output On.
17. Enter the Mean measurement value in the test record.
18. Double-tap the channel under test badge to open its configuration menu and change the **Offset** to **-900 mV**.
19. Set the calibrator output to **-900 mV**, as shown in the test record.
20. Enter the Mean measurement value in the test record.
21. Repeat step 15 on page 123 through 20 on page 123, changing the channel vertical settings and the calibrator output as listed in the test record for the channel under test.
22. Repeat the channel tests at 1 M $\Omega$  impedance.
  - a. Set the calibrator output to Off or 0 volts.
  - b. Change the calibrator impedance to **1 M $\Omega$**  and voltage to **+900 mV**.
  - c. Turn the calibrator output On.
  - d. Repeat steps 15 on page 123 through 20 on page 123, changing the channel **Termination** to **1 M $\Omega$**  and the vertical Offset value and the calibrator output as listed in the 1 M $\Omega$  test record for the channel under test.
23. Repeat the procedure for all remaining channels.
  - a. Double-tap the **Mean** measurement badge.
  - b. Tap the **Configure** panel.
  - c. Tap the **Source 1** field and select the next channel to test.
  - d. Set the calibrator to **0** volts and **50  $\Omega$**  output impedance.
  - e. Move the calibrator output to the next channel input to test.
  - f. Double-tap the channel badge of the channel that you have finished testing and set **Display** to **Off**.
  - g. Tap the channel button on the oscilloscope Settings bar of the next channel to test.
  - h. Starting from step 2 on page 122 , repeat the procedure until all channels have been tested.

## Check analog bandwidth

This test checks the bandwidth at 50  $\Omega$  and 1 M $\Omega$  terminations for each channel. The typical bandwidth at 1 M $\Omega$  termination is checked on the products as a functional check.

1. Connect the output of the calibrated leveled sine wave generator to the oscilloscope channel 1 input as shown in the following illustration.

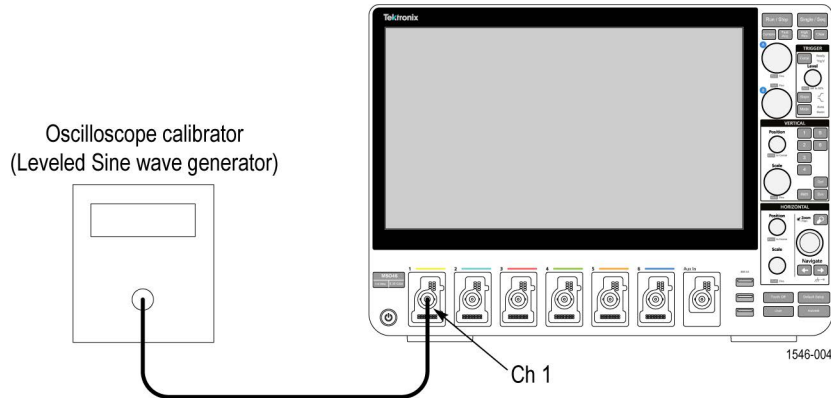

**WARNING:** Set the generator to off or 0 volts before connecting, disconnecting, and/or moving the test hookup during the performance of this procedure. The generator is capable of providing dangerous voltages.

2. Tap **File > Default Setup** to reset the instrument and add the channel 1 badge and signal to the display.
3. Add the peak-to-peak measurement.
  - a. Tap the **Add New. Measure** button.
  - b. Set the **Source** to the channel under test.
  - c. In the **Amplitude Measurements** panel, double-tap the **Peak-to-Peak** measurement button to add the measurement badge to the Results bar.
  - d. Tap outside the menu to close it.
  - e. Double-tap the **Peak-to-Peak** results badge.
  - f. Tap **Show Statistics in Badge**.
  - g. Tap **FILTER/LIMIT RESULTS** to open the panel.
  - h. Tap **Limit Measurement Population** to toggle it to **On**.
  - i. Tap outside the menu to close it.
4. Set the channel under test settings:
  - a. Double-tap the badge of the channel under test to open its configuration menu.
  - b. Set **Vertical Scale** to **1 mV/div**.
  - c. Set **Termination** to **50  $\Omega$** .
  - d. Tap outside the menu to close it.
5. Adjust the leveled sine wave signal source to display a waveform of 8 vertical divisions at the selected vertical scale with a set frequency of **10 MHz**. For example, at 5 mV/div, use a  $\geq 40$  mV<sub>p-p</sub> signal; at 2 mV/div, use a  $\geq 16$  mV<sub>p-p</sub> signal.



**Note:** At some V/div settings, the generator may not provide 8 vertical divisions of signal. Set the generator output to obtain as many vertical divisions of signal as possible.

6. Double-tap the **Horizontal** badge in the Settings bar.
7. Set the **Horizontal Scale** to **1 ms/division**.
8. Tap outside the menu to close it.
9. Record the **Peak-to-Peak** measurement in the **V<sub>in-pp</sub>** entry of the test record.

10. Double-tap the **Horizontal** badge in the Settings bar.
11. Set the **Horizontal Scale** to **4 ns/division**.
12. Adjust the signal source to the maximum bandwidth frequency for the bandwidth and model being tested.
13. Record the peak-to-peak measurement.
  - a. Record the **Peak-to-Peak** measurement at the new frequency in the  $V_{bw-pp}$  entry of the test record.
14. Use the values of  $V_{bw-pp}$  and  $V_{in-pp}$  recorded in the test record, and the following equation, to calculate the Gain at bandwidth:  

$$Gain = V_{bw-pp} / V_{in-pp}$$

To pass the performance measurement test, Gain should be  $\geq 0.707$ . Enter *Gain* in the test record.
15. Repeat steps 4 on page 124 through 14 on page 125 for all combinations of Vertical Scale settings listed in the test record.
16. Repeat the tests at 1 M $\Omega$  impedance.
  - a. Set the calibrator output to Off or 0 volts.
  - b. Change the calibrator impedance to **1 M $\Omega$** .
  - c. Double-tap the badge of the channel under test to open its menu.
  - d. Set the **Termination** to **1 M $\Omega$** .
  - e. Repeat steps 4 on page 124 through 16 on page 125, but leave the termination set to **1 M $\Omega$** .
17. Repeat the test for all remaining channels.
  - a. Set the calibrator to **0** volts and **50  $\Omega$**  output impedance.
  - b. Move the calibrator output to the next channel input to be tested.
  - c. Double-tap the channel badge of the channel that you have finished testing and set **Display** to **Off**.
  - d. Tap the channel button on the oscilloscope Settings bar of the next channel to test.
  - e. Double-tap the **Peak-to-Peak** measurement badge.
  - f. Tap the **Configure** panel.
  - g. Tap the **Source 1** field and select the next channel to test.
  - h. Starting from step 4 on page 124, repeat the procedure until all channels have been tested.

## Check random noise

This test checks random noise at 1 M $\Omega$  and 50  $\Omega$  for each channel, in HiRes acquisition mode. You do not need to connect any test equipment to the oscilloscope for this test.

1. Disconnect everything from the oscilloscope inputs.
2. Tap **File > Default Setup**.
3. Turn on **HiRes** Mode except for 1.5 GHz instruments. 1.5 GHz instruments must be tested in **Sample** mode.
4. Add the **AC RMS** measurement:
  - a. Tap the **Add New... Measure** button.
  - b. Set the **Source** to the channel being tested.
  - c. In the **Amplitude Measurements** panel, double-tap the **AC RMS** measurement button to add the measurement badge to the Results bar.
  - d. Tap outside the menu to close it.
  - e. Double-tap the **AC RMS** measurement badge and tap **Show Statistics in Badge** to display statistics in the measurement badge.
  - f. Tap the **Filter / Limit Results** panel.
  - g. Turn on **Limit Measurement Population**.
  - h. Set the limit to **100**.


- i. Tap outside the menu to close it.
5. Set up the Horizontal mode:
  - a. Double-tap the **Horizontal** setting badge.
  - b. Set **Horizontal Mode** to **Manual**.
  - c. Set the **Sample Rate** to **6.25 GS/s**.
  - d. Set the **Record Length** to **2 Mpts**.
  - e. Tap outside the menu to close it.
6. Double-tap the Channel badge of the channel being tested.
7. Set the **Vertical Scale** value to **1 mV**.
8. Check **1 M  $\Omega$**  termination.
  - a. In the Channel badge menu, tap **1 M  $\Omega$**  termination.
  - b. Tap the **Bandwidth Limit** field and select the highest frequency listed.
  - c. Set the channel **Position** value to **340 mdivs**.
  - d. Once the measurement count (N) in the AC RMS measurement badge reaches 100, record the AC RMS Mean value (the  $\mu$  readout).
  - e. Set the channel vertical **Position** value to **360 mdivs**.
  - f. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the  $\mu$  readout).
  - g. Average the two values and record the result in the **1 mV/div > Full** row of the **1 M $\Omega$**  column of the Test Result record.
  - h. In the channel badge menu, tap the **Bandwidth Limit** field and select **250 MHz**.
  - i. Set the channel vertical **Position** value to **340 mdivs**.
  - j. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the  $\mu$  readout).
  - k. Set the channel vertical Position value to **360 mdivs**.
  - l. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the  $\mu$  readout).
  - m. Average the two values and record the result in the **1 mV/div > 250MHz limit** row of the **1 M $\Omega$**  column of the Test Result record.
  - n. Tap the **Bandwidth Limit** field and select **20 MHz**.
  - o. Set the channel vertical **Position** value to **340 mdivs**.
  - p. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the  $\mu$  readout).
  - q. Set the channel vertical **Position** value to **360 mdivs**.
  - r. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the  $\mu$  readout).
  - s. Average the two values and record the result in the **1 mV/div > 20MHz limit** row of the **1 M $\Omega$**  column of the Test Result record.
9. Check **50  $\Omega$**  termination.
  - a. In the Channel badge, set **Termination** to **50  $\Omega$** .
  - b. Tap the **Bandwidth Limit** field and select the highest frequency listed.
  - c. Set the channel vertical Position value to **340 mdivs**.
  - d. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the  $\mu$  readout).
  - e. Set the channel vertical Position value to **360 mdivs**.
  - f. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the  $\mu$  readout).
  - g. Average the two values and record the result in the **1 mV/div > Full** row of the **50  $\Omega$**  column of the Test Result record.
  - h. Tap the **Bandwidth Limit** field and select **250 MHz**.
  - i. Set the channel vertical **Position** value to **340 mdivs**.
  - j. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the  $\mu$  readout).
  - k. Set the channel vertical **Position** value to **360 mdivs**.
  - l. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the  $\mu$  readout).

- m. Average the two values and record the result in the **1 mV/div > 250MHz limit** row of the **50 Ω** column of the Test Result record.
  - n. Tap the **Bandwidth Limit** field and select **20 MHz**.
  - o. Set the channel vertical **Position** value to **340 mdivs**.
  - p. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the **μ** readout).
  - q. Set the channel vertical **Position** value to **360 mdivs**.
  - r. Once the measurement count (N) in the measurement badge reaches 100, record the AC RMS Mean value (the **μ** readout).
  - s. Average the two values and record the result in the **1 mV/div > 20MHz limit** row of the **50 Ω** column of the Test Result record.
10. Repeat 1 MΩ and 50 Ω tests at all V/div settings for the current channel.
- a. In the Channel badge, set the **Vertical Scale** setting to the next value in the test record (2 mV, 5 mV, and so on, up to 1 V/div).
  - b. Repeat steps 8 on page 126 through 9 on page 126.
11. Repeat all tests for the remaining input channels.
- a. Double-tap the **AC RMS** measurement badge.
  - b. Tap the **Configure** panel.
  - c. Tap the **Source 1** field and select the next channel to test.
  - d. Double-tap the channel badge of the channel that you have finished testing and set **Display** to **Off**.
  - e. Tap the channel button on the oscilloscope Settings bar of the next channel to test.
  - f. Double-tap the channel badge for the channel being tested.
  - g. Starting at step 7 on page 126, repeat these procedures for each input channel.

## Check long term sample rate

This test checks the sample rate and delay time accuracy (time base).

1. Connect the output of a time mark generator to the oscilloscope channel 1 input using a 50 Ω cable, as shown in the following illustration.

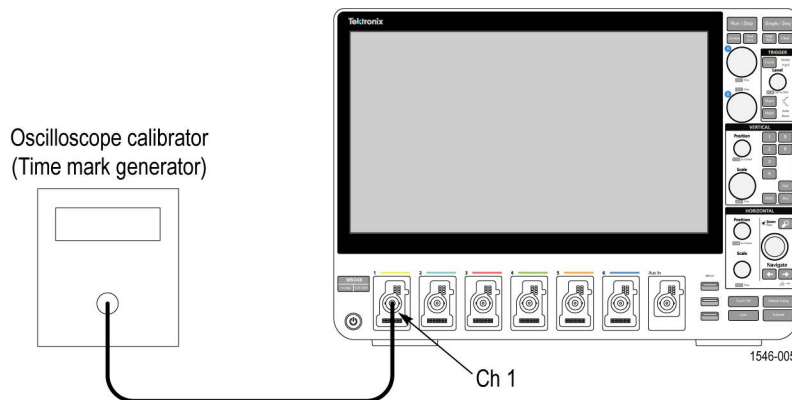

**WARNING:** Set the generator output to off or 0 volts before connecting, disconnecting, and/or moving the test hookup during the performance of this procedure. The generator is capable of providing dangerous voltages.

2. Set the time mark generator period to **80 ms**. Use a time mark waveform with a fast rising edge.
3. If it is adjustable, set the time mark amplitude to approximately **2 V<sub>p-p</sub>**.
4. Tap **File > Default Setup**.
5. Tap the channel **1** button on the Settings bar.
6. Double-tap the Channel 1 badge to open its Configuration menu.
7. Set **Termination** to **50 Ω**.

8. Set **Vertical Scale** to **500 mV**.
9. Set the **Position** value to center the time mark signal on the screen.
10. Tap outside the menu area to close it.
11. Double-tap the **Horizontal** settings badge.
12. Set the **Horizontal Scale** to **100 ns/div**.
13. Tap outside the menu area to close it.
14. Double-tap the **Trigger** settings badge.
15. Set **Source** to the channel being tested.
16. Set the **Level** as necessary for a triggered display.
17. Tap outside the menu area to close it.
18. Double-tap the **Horizontal** settings badge.
19. Adjust the **Position** value to move the trigger point to the center of the screen.
20. Turn **Delay** to **On** and set **Position** to **80 ms**.
21. Set the **Horizontal Scale** to **100 ns/div**.
22. Observe where the rising edge of the marker crosses the center horizontal graticule line. The rising edge should cross within  $\pm 2$  divisions of the vertical center graticule. Enter the deviation in the test record.



**Note:** A  $2.5 \times 10^{-6}$  time base error is 2 divisions of displacement.


## Check digital threshold accuracy

This test checks the threshold accuracy of the TLP058 logic probe digital channels D0-D7 at 0 V and 25 °C, for all oscilloscope input channels.



**Note:** Threshold Accuracy is a function of the logic probe only. It is a typical specification. The Threshold Accuracy test checks the typical logic probe performance, and may be considered a functional check of the oscilloscope digital input.

1. Connect a TLP058 digital probe to channel 1.

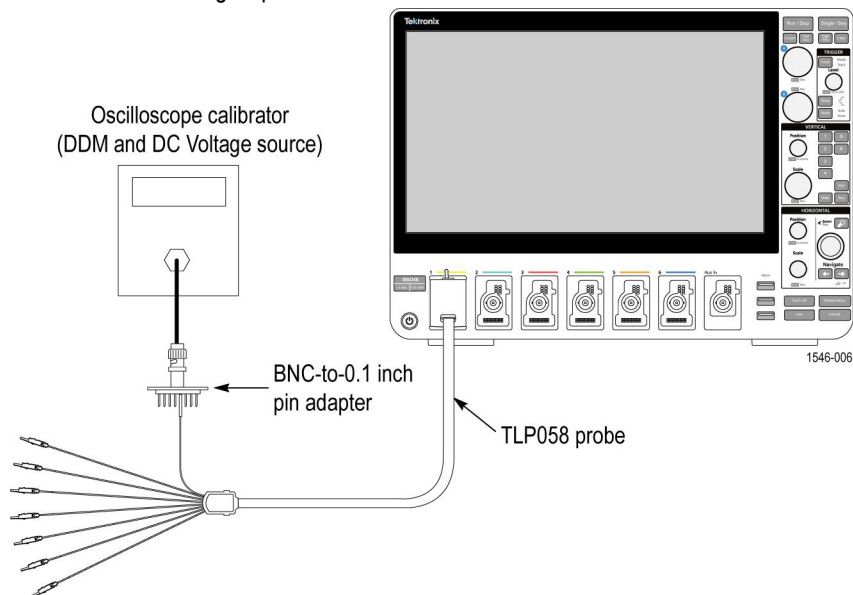

2. Connect the DC voltage source to digital channel **D0**.





**WARNING:** Set the generator output to Off or 0 volts before connecting, disconnecting, or moving the test hookup during the performance of this procedure. The generator is capable of providing dangerous voltages.

If you are using the Fluke 9500 calibrator as the DC voltage source, connect the calibrator head to the digital channel D0, using the BNC-to-0.1 inch pin adapter listed in the *Required equipment* table. Be sure to connect channel D0 to both the corresponding signal pin and to a ground pin on the adapter.

3. Tap **File > Default Setup**. This resets the instrument and adds the channel 1 badge and signal to the display.
4. Display the digital channels and set the thresholds.
  - a. Double-tap the badge of the channel under test on the Settings bar.
  - b. Double-tap the **Threshold** field at the bottom of the menu and set the value to **0 V**.
  - c. Tap **Set All Thresholds**. All thresholds are now set for the 0 V threshold check.
  - d. Tap outside the menu to close it.

5. Double-tap the **Horizontal** badge in the Settings bar.

6. Set the **Horizontal Scale** to **10 ns/div**.

7. Tap outside the menu to close it.

8. Set the calibrator DC voltage output ( $V_s$ ) to **-400 mV**.

9. Wait 1 second. Verify that the logic level is low on **D0**.

10. Increment  $V_s$  by **+10 mV**. Wait 1 second and check the logic level of the channel D0 signal display.

If the signal level is a logic low or is alternating between high and low, continue to increment  $V_s$  by +10 mV, wait 1 second, and check the logic level until the logic state is a steady high.

11. Record this  $V_s$  value as **Vs-** for D0 of the test record.

12. Double-tap the **Trigger** badge and set the **Slope** to **Falling** edge.

13. Set the DC voltage source ( $V_s$ ) to **+400 mV**.

14. Wait 1 second. Verify that the logic level is high.

15. Decrement  $V_s$  by **-10 mV**. Wait 1 second and check the logic level of the channel D0 signal display.

If the signal level is a logic high or is alternating between high and low, continue to decrement  $V_s$  by -10 mV, wait 1 second, and check the logic level until the logic state is a steady low.

16. Record this  $V_s$  value as **Vs+** for D0 of the test record.

17. Find the average using this formula:  $V_{sAvg} = (V_{s-} + V_{s+})/2$ .

18. Record the average as the test result for D0 in the test record. The test result should be between the low and high limits.

19. Repeat the procedure for all remaining digital channels.

- a. Connect the next digital channel to be tested (D1, D2, and so on) to the DC voltage source.
- b. Repeat steps 8 on page 129 through 19 on page 129, until all digital channels have been tested for this input channel.


20. Repeat the procedure for all remaining input channels.

- a. Move the TLP058 digital probe from channel 1 to channel 2.
- b. Set the generator output to 0 volts and Off.
- c. Repeat steps starting at 2 on page 128 for the channel being tested (channel 2, channel 3, and so on).

## Check AUX Out output voltage levels

This test checks the output voltage levels from the AUX Out connector.

1. Use a 50  $\Omega$  cable to connect the AUX Out signal from the rear of the instrument to the channel 1 input of the same instrument, as shown in the following illustration.

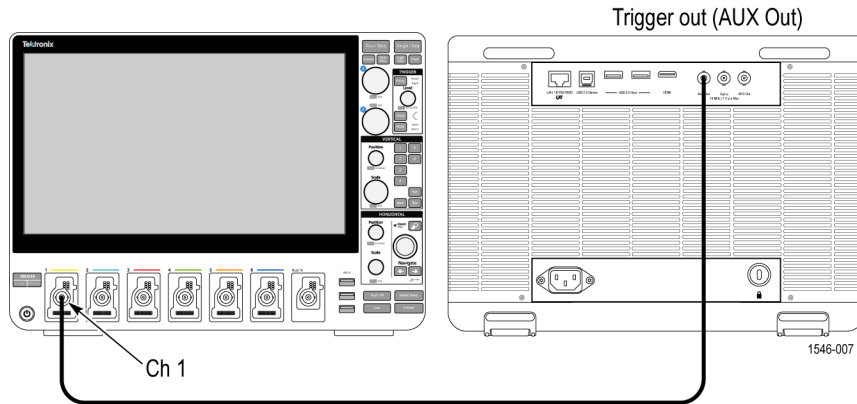


2. Tap **File > Default Setup**. This resets the instrument and adds the channel 1 badge and signal to the display.
3. Double-tap the badge of the channel 1 badge to open its configuration menu.
4. Set the **Vertical Scale** to **1 V/div**.
5. Tap outside the menu to close it.
6. Double-tap the **Horizontal** badge in the Settings bar.
7. Set the **Horizontal Scale** to **400 ns/div**.
8. Tap outside the menu to close it.
9. Record the Maximum and Minimum measurements at 1 M $\Omega$  termination.
  - a. Tap the **Add New... Measure** button.
  - b. In the Amplitude Measurements panel, set the **Source** to **Ch 1**.
  - c. Double-tap the **Maximum** button to add the measurement badge to the Results bar.
  - d. Double-tap the **Minimum** button to add the measurement badge to the Results bar.
  - e. Tap outside the menu to close it.
  - f. Double-tap the **Maximum** results badge.
  - g. Tap **Show Statistics in Badge**.
  - h. Tap **FILTER/LIMIT RESULTS** to open the panel.
  - i. Tap **Limit Measurement Population** to toggle it to **On**.
  - j. Tap outside the menu to close it.
  - k. Double-tap the **Minimum** results badge.
  - l. Tap **Show Statistics in Badge**.
  - m. Tap **FILTER/LIMIT RESULTS** to open the panel.
  - n. Tap **Limit Measurement Population** to toggle it to **On**.
  - o. Tap outside the menu to close it.
  - p. Enter the Maximum and Minimum measurement readings in the 1 M $\Omega$  row of the test record.
10. Record the Maximum and Minimum measurements at 50  $\Omega$  termination.
  - a. Double-tap the **Ch 1** badge to open its configuration menu.
  - b. Set **Termination** to **50  $\Omega$** .
  - c. Tap outside the menu to close it.
  - d. Enter the Maximum and Minimum measurement readings in the 50  $\Omega$  row of the test record.

## Check DVM voltage accuracy (DC)

This test checks the DC voltage accuracy of the Digital Volt Meter (DVM) option. The DVM option is available for free when you register the instrument at tek.com.

### Procedure

1. Connect the oscilloscope to a DC voltage source to run this test. If using the Fluke 9500 calibrator as the DC voltage source, connect the calibrator head to the oscilloscope channel to test.

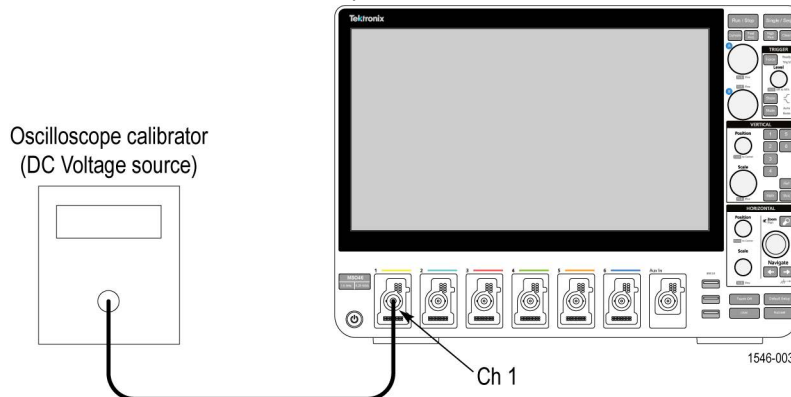

**WARNING:** Set the generator output to Off or 0 volts before connecting, disconnecting, or moving the test hookup during the performance of this procedure. The generator is capable of providing dangerous voltages.


2. Set the calibrator impedance to **1 MΩ**.
3. Tap **File > Default Setup**. This resets the instrument and adds the channel 1 badge and signal to the display.
4. Set the channel settings.
  - a) Double tap the badge of the channel under test to open its menu.
  - b) Check that **Position** is set to **0 divs**. If not, set the position to 0 divisions.
  - c) Confirm that **Termination** is set to **1 MΩ**.
  - d) Set the **Bandwidth Limit** to **20 MHz**.
5. Set the calibrator impedance to **1 MΩ**.
6. Double-tap the **Horizontal** badge and set **Horizontal Scale** to **1 ms/div**.
7. Tap outside the menu to close it.
8. Double-tap the **Acquisition** badge and set the **Acquisition Mode** to **Average**.
9. Verify or set the **Number of Waveforms** to **16**.
10. Tap outside the menu to close it.
11. Double-tap the **Trigger** badge and set the **Source** to **AC Line**.
12. Tap outside the menu to close it.
13. Tap the **DVM** button to add the DVM badge to the Results bar.
14. In the **DVM** menu, set **Source** to the channel to be tested.
15. Set **Mode** to **DC**.
16. Tap outside the menu to close it.
17. Set the calibrator to the input voltage shown in the test record (for example, **-5 V** for a **1V/div** setting).
18. In the channel under test menu, set the **Offset** value to that shown in the test record (for example, **-5 V** for **-5 V** input and **1 V/div** setting).
19. Set the **Vertical Scale** field to match the value in the test record (for example, **1 V/div**).
20. Enter the measured value on the DVM badge into the DVM Voltage Accuracy Tests record.

21. Repeat the procedure (steps 17 on page 131, 18 on page 131, 19 on page 131 and 20 on page 131) for each volts/division setting shown in the test record.
22. Repeat all steps, starting with step 4 on page 131, for each oscilloscope channel to check. To set the next channel to test:
  - a) Double tap the badge of the channel under test to open its menu.
  - b) Set **Display** to **Off**.
  - c) Tap the channel button in the Settings bar of the next channel to test to add that channel badge and signal to the display.

## Check DVM voltage accuracy (AC)

This test checks the AC voltage accuracy of the Digital Volt Meter (DVM) option. The DVM option is available for free when you register the instrument at tek.com.

### Procedure

1. Connect the output of the leveled square wave generator (for example, Fluke 9500) to the oscilloscope channel 1 input.  
 **WARNING:** Set the generator output to Off or 0 volts before connecting, disconnecting, or moving the test hookup during the performance of this procedure. The generator is capable of providing dangerous voltages.
2. Set the generator to **50  $\Omega$**  output impedance (50  $\Omega$  source impedance).
3. Set the generator to produce a square wave of the amplitude and frequency listed in the test record (for example, 20 mV<sub>pp</sub> at 1 kHz).
4. Tap **File > Default Setup** to reset the instrument and add the channel 1 badge and signal to the display.
5. Tap the **DVM** button to add the DVM badge to the Results bar.
6. Set the DVM **Mode** to **AC RMS**.
7. In the DVM menu, set **Source** to the channel to be tested.
8. Double-tap the channel badge of the channel being tested to open its configuration menu.
9. Set **Termination** to **50  $\Omega$** .
10. Use the **Vertical Scale** controls to set the signal height so that the signal covers between 4 and 8 vertical divisions on the screen.
11. Enter the DVM measured value in the test record.
12. Repeat steps 10 on page 132 and 11 on page 132 for each voltage and frequency combination shown in the record.
13. Repeat all steps to test all remaining oscilloscope channels. To set the next channel to test:
  - a) Double tap the badge of the channel under test to open its menu.
  - b) Set **Display** to **Off**.
  - c) Tap the channel button in the Settings bar of the next channel to test to add that channel badge and signal to the display.

## Check trigger frequency accuracy and maximum input frequency

This test checks trigger frequency counter accuracy. The trigger frequency counter is part of the free DVM and trigger frequency option that is available when you register the instrument at tek.com.

### Procedure

1. Tap **File > Default Setup** to reset the instrument and add the channel 1 badge and signal to the display.
2. Connect the **10 MHz Reference out** from the time mark generator to the **Ref In** connector on the back of the oscilloscope.
3. Connect the output of the time mark generator to the oscilloscope channel input being tested using a 50  $\Omega$  cable. Set the time mark generator to a 50  $\Omega$  source and a fast rising edge waveform ( $\geq 3$  mV/ns).
4. Set the time mark generator frequency to the first value shown in the test record, starting at **100 Hz**.
5. Set the mark amplitude to **1 V<sub>pp</sub>**, which makes a 2 divisions high waveform.

6. Double-tap the channel badge being tested (starting with channel 1) and set **Termination** to **50  $\Omega$** .
7. Set the channel **Vertical Scale** to **500 mV/div**.
8. Tap outside the menu to close it.
9. Double-tap the **Acquisition** badge and set the **Timebase Reference Source** to **External (10 MHz)**.
10. Tap outside the menu to close it.
11. Double-tap the **Horizontal** badge and use the **Horizontal Scale** controls to display at least 2 cycles of the waveform.
12. Tap outside the menu to close it.
13. Double-tap the **Trigger** badge to open its menu.
  - a) Set the **Source** field to the input channel being tested.
  - b) Tap the **Set to 50%** button to obtain a stable display.
  - c) Tap the **Mode & Holdoff** panel to open the **Mode & Holdoff** configuration menu.
  - d) In the **Mode & Hold Off** menu, set the **Trigger Frequency Counter** to **On**. The trigger frequency readout is at the bottom of the **Trigger** badge.
  - e) Tap outside the menu to close it.
14. Double-tap the channel badge being tested (starting with channel 1) and use the **Position** controls to vertically center the time mark in the waveform graticule.
15. Enter the value of the trigger frequency (**F** readout in the **Trigger** badge) in the test record for that frequency.
16. Repeat this procedure for each frequency setting shown in the record. Make sure to adjust the Horizontal scale after each calibrator frequency change to show at least two cycles of the waveform on the screen.
17. Repeat all these steps to test each oscilloscope channel.

## Check AFG sine and ramp frequency accuracy

This test verifies the frequency accuracy of the arbitrary function generator. All output frequencies are derived from a single internally generated frequency. Only one frequency point of channel 1 is required to be checked.

1. Connect a 50  $\Omega$  cable from the **AFG Out** connector to the frequency counter input as shown in the following figure.

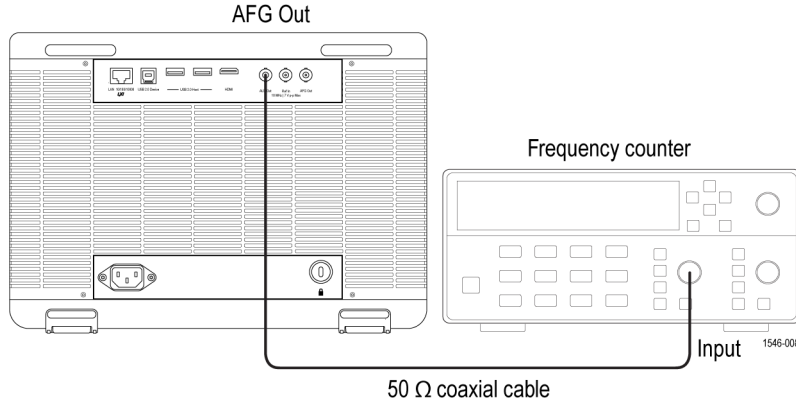


Figure 1: Frequency/period test

2. Tap **File > Default Setup** to set the instrument to the factory default settings.
3. Tap the **AFG** button to open the **AFG** menu.
4. Set the arbitrary function generator output as follows:

Select menu	Setting
Output	On
Waveform Type	Sine
Frequency	1.000000 MHz
Amplitude	1.00 V <sub>PP</sub>

5. Turn on the frequency counter:
  - a. Double-tap the **Trigger** badge to open its menu.
  - b. Set the **Source** field to the input channel being tested.
  - c. Tap the **Set to 50%** button to obtain a stable display.
  - d. Tap the **Mode & Holdoff** panel to open the **Mode & Holdoff** configuration menu
  - e. In the **Mode & Holdoff** menu, set the **Trigger Frequency Counter** to **On**. The trigger frequency readout is at the bottom of the **Trigger** badge.
  - f. Tap outside the menu to close it.
6. Check that the reading of the frequency counter is between **0.999950 MHz** and **1.000050 MHz**. Enter the value in the Test record.
7. Set the arbitrary function generator output as follows:

Select menu	Setting
Waveform Type	Ramp
Frequency	500 kHz

8. Check that reading of the frequency counter is between **499.975 kHz** and **500.025 kHz**. Enter the value in the Test record.

## Check AFG square and pulse frequency accuracy

This test verifies the frequency accuracy of the arbitrary function generator. All output frequencies are derived from a single internally generated frequency. Only one frequency point of channel 1 is required to be checked.

1. Connect the arbitrary function generator to the frequency counter as shown in the following figure.

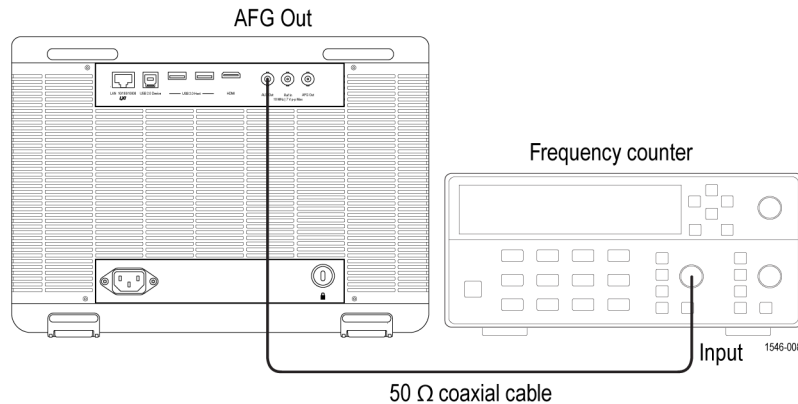


Figure 2: Frequency/period test

2. Tap **File > Default Setup** to set the instrument to the factory default settings.
3. Tap the **AFG** button to open the AFG menu.
4. Set the arbitrary function generator as follows:

Select menu	Setting
Waveform Type	Square
Frequency	1.000000 MHz
Amplitude	1.00 V <sub>PP</sub>
Output	On

5. Turn on the frequency counter:
  - a. Double-tap the **Trigger** badge to open its menu.
  - b. Set the **Source** field to the input channel being tested.
  - c. Tap the **Set to 50%** button to obtain a stable display.
  - d. Tap the **Mode & Holdoff** panel to open the **Mode & Holdoff** configuration menu
  - e. In the **Mode & Holdoff** menu, set the **Trigger Frequency Counter** to **On**. The trigger frequency readout is at the bottom of the **Trigger** badge.
  - f. Tap outside the menu to close it.
6. Check that the frequency counter readout is between **0.999950 MHz** and **1.00005 MHz**. Enter the value in the Test record.
7. Set up the arbitrary function generator as follows:

Select menu	Setting
Waveform Type	Pulse

8. Check that reading of the frequency counter is between **0.999950 MHz** and **1.000050 MHz**. Enter the value in the Test record.

## Check AFG signal amplitude accuracy

This test verifies the amplitude accuracy of the arbitrary function generator. All output amplitudes are derived from a combination of attenuators and 3 dB variable gain. Some amplitude points are checked. This test uses a 50 Ω terminator. It is necessary to know the accuracy of the 50 Ω terminator in advance of this amplitude test. This accuracy is used as a calibration factor.

1. Connect the 50 Ω terminator to the DMM as shown in the following figure and measure the resistance value.

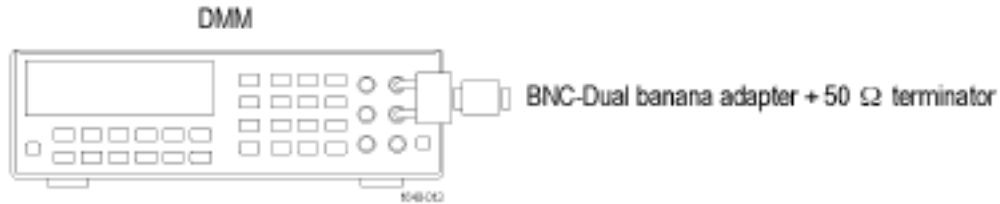


Figure 3: 50 Ω terminator accuracy

2. Calculate the 50 Ω calibration factor (CF) from the reading value and record as follows:

**Table 2: CF (Calibration Factor) = 1.414 × ((50 / Measurement Ω) + 1)**

Measurement (reading of the DMM)	Calculated CF

Examples:

- For a measurement of 50.50 Ω, CF = 1.414 ( 50 / 50.50 + 1) = **2.814**.
  - For a measurement of 49.62 Ω, CF = 1.414 ( 50 / 49.62 + 1) = **2.839**.
3. Connect the arbitrary function generator output to the DMM as shown in the following figure. Be sure to connect the 50 Ω terminator to the **AFG Out** connector.

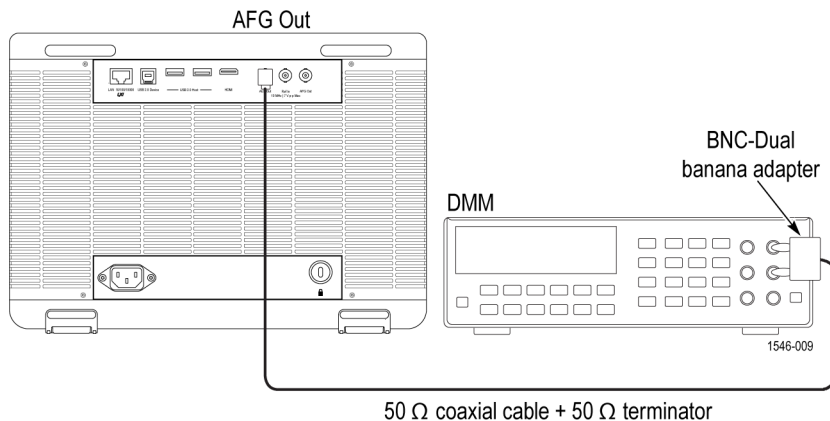


Figure 4: Amplitude test

4. Tap the **AFG** button and set up the arbitrary function generator output as follows:

Select menu	Setting
Waveform Type	Sine
Frequency	1.000000 kHz
Amplitude	30 mV <sub>PP</sub>
Load Impedance	50 Ω
Table continued...	



Select menu	Setting
Output	On

- Measure the **AC RMS** voltage readout on the DMM.
- Multiply the DMM voltage by the calculated CF to get the corrected peak to peak voltage. Enter the resulting value in the Measurement field in the following table.
- Change the AFG output amplitude to the next value in the table.
- Repeat steps 5 on page 137 through 7 on page 137 for each amplitude value. Check that the peak to peak voltages are within the limits in the table below. Enter the values in the test record.

Waveform Type	Frequency	Amplitude	Measurement	Range
Sine	1.000 kHz	30.0 mV <sub>PP</sub>		28.55 mV <sub>PP</sub> - 31.45 mV <sub>PP</sub>
Sine	1.000 kHz	300.0 mV <sub>PP</sub>		294.5 mV <sub>PP</sub> - 305.5 mV <sub>PP</sub>
Sine	1.000 kHz	800.0 mV <sub>PP</sub>		787.0 mV <sub>PP</sub> - 813.0 mV <sub>PP</sub>
Sine	1.000 kHz	1.500 V <sub>PP</sub>		1.4765 V <sub>PP</sub> - 1.5235 V <sub>PP</sub>
Sine	1.000 kHz	2.000 V <sub>PP</sub>		1.969 V <sub>PP</sub> - 2.031 V <sub>PP</sub>
Sine	1.000 kHz	2.500 V <sub>PP</sub>		2.4615 V <sub>PP</sub> - 2.5385 V <sub>PP</sub>

## Check AFG DC offset accuracy

This test verifies the DC offset accuracy of the arbitrary function generator. This test uses a 50 Ω terminator. It is necessary to know the accuracy of the 50 Ω terminator in advance of this test. This accuracy is used as a calibration factor.

- Connect the 50 Ω terminator to the DMM as shown in the following figure and measure the resistance value.



Figure 5: 50 Ω terminator accuracy

- Calculate the 50 Ω calibration factor (CF) from the reading value and record as follows:

**Table 3: CF (Calibration Factor) =  $0.5 \times ((50 / \text{Measurement } \Omega) + 1)$**

Measurement (reading of the DMM)	Calculated CF

Examples:

- For a measurement of 50.50 Ω, CF =  $0.5 (50 / 50.50 + 1) = \mathbf{0.9951}$ .
- For a measurement of 49.62 Ω, CF =  $0.5 (50 / 49.62 + 1) = \mathbf{1.0038}$ .

3. Connect the arbitrary function generator output to the DMM as shown in the following figure. Be sure to connect the 50 Ω terminator to the arbitrary function generator **AFG Output** connector.

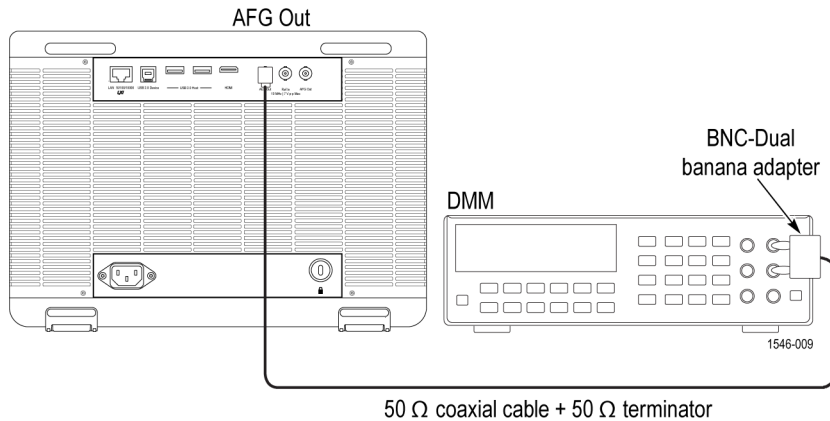


Figure 6: DC offset tests

4. Tap the **AFG** button and set up the arbitrary function generator as follows:

Select menu	Setting
Waveform Type	DC
Offset	+ 1.25 V
Output	On

5. Measure the voltage readout on the DMM.
6. Multiply the DMM voltage by the calculated CF to get the corrected offset voltage. Enter the resulting value in the Measurement field in the following table.

Function	Offset	Measurement	Range
DC	+ 1.25 Vdc	Vdc	1.23025 Vdc to 1.26975 Vdc
DC	0.000 Vdc	Vdc	- 0.001 Vdc to + 0.001 Vdc
DC	- 1.25 Vdc	Vdc	-1.26975 Vdc to -1.23025 Vdc

7. Change the AFG output amplitude to the next value in the table, measure the voltage readout on the DMM, multiply the DMM readout by the calculated CF to get the corrected offset voltage, and enter the resulting value in the Measurement field in the table.
8. Verify that the corrected offset measurements are within the range.