

HC5
Transit Case
Instructions


Revision A

Transit case description

The HC5 is a ruggedized, waterproof and dust tight (MIL-C-4150J) transit case specifically designed to provide travel and storage protection for the 5/6 Series MSO instruments.

The case protects instruments from shock, vibration, and moisture. The case also has room for the accessories pouch (for probes, adapters, and manuals).

Other features include an automatic air pressure equalization control valve for use during air transport, and security rings for use with locks (locks not included).

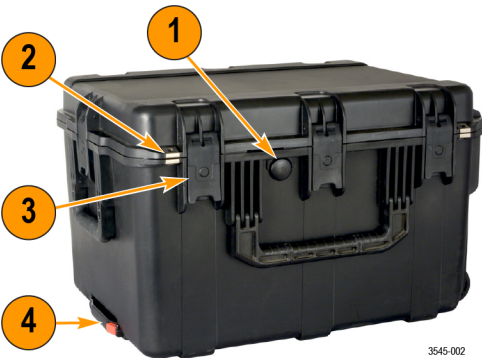

- 1. Automatic air pressure valve
- 2. Security rings (two)
- 3. Latches (five)
- 4. Extending handle

Specification	Description		
Material	Ultra-High Impact Polypropylene/Black, Polyurethane foam lining		
Shipping Weight (with foam)	24.62 lbs. (11.17 kg)		
Exterior Dimensions	Length	Width	Height
	25.63 inches (65.09 cm)	19.50 inches (49.53 cm)	15.63 inches (39.69 cm)

Safely rotate the handle



Use the correct process to eliminate the chance of pinching your thumb or rear-panel-connected cables while rotating the handle.



WARNING: Hold the top of the handle to rotate the handle on the instrument. Do not hold the handle from the sides and rotate, as this can pinch the base of your thumb between the handle and the case.



CAUTION: If you have routed any cables between the handle and the case, be careful when rotating the handle so that you do not pinch the cables.

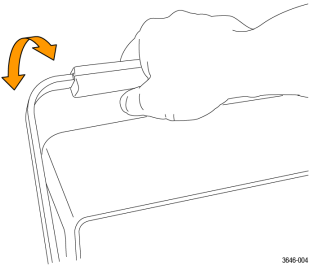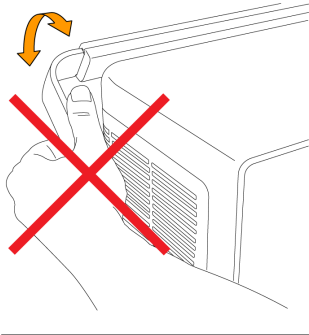

Packing instructions

Use these instructions to install the hard cover, pack the instrument, and unpack the instrument.

The transit case consists of a heavy duty outer shell and an inner layer of foam. The inner foam consists of a permanent ring of foam and one removable foam piece.


Install the cover

Remove the pouch from the front cover and install the hard cover on the instrument.



Pack the instrument

1. Remove the foam piece and pack the instrument (with hard cover attached) rear panel first.
2. Put the foam back on top of the instrument.

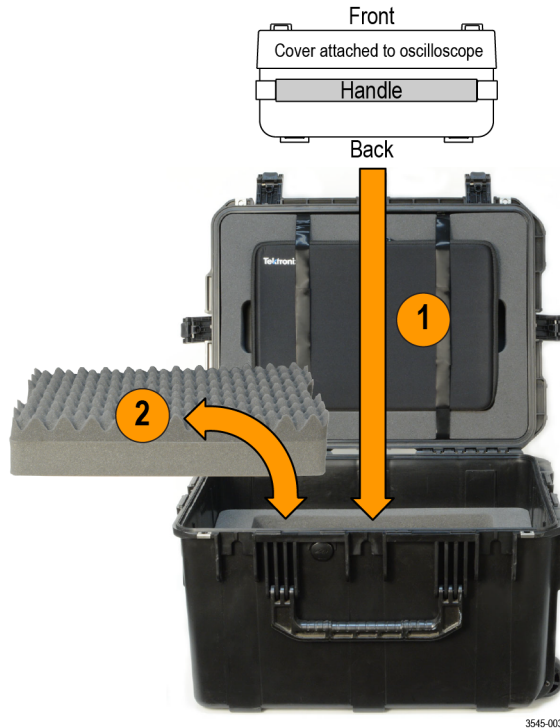

Unpack the instrument

To remove the oscilloscope from the case, grab the handle and pull and rotate the oscilloscope up and out from the foam liner.

Copyright © 2023, Tektronix. 2023 All rights reserved. Licensed software products are owned by Tektronix or its subsidiaries or suppliers, and are protected by national copyright laws and international treaty provisions. Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specifications and price change privileges reserved. All other trade names referenced are the service marks, trademarks, or registered trademarks of their respective companies.

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

Tektronix, Inc.
14150 SW Karl Braun Drive
P.O. Box 500
Beaverton, OR 97077
US

For product information, sales, service, and technical support visit tek.com to find contacts in your area. For warranty information visit tek.com/warranty.