

**RSA5115A and RSA5126A
Real Time Signal Analyzers
Option 51 Preamp Upgrade
Instructions**

www.tek.com



071-3094-00

Tektronix

Copyright © Tektronix. All rights reserved. Licensed software products are owned by Tektronix or its subsidiaries or suppliers, and are protected by national copyright laws and international treaty provisions.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specifications and price change privileges reserved.

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

Contacting Tektronix

Tektronix, Inc.
14150 SW Karl Braun Drive
P.O. Box 500
Beaverton, OR 97077
USA

For product information, sales, service, and technical support:

- In North America, call 1-800-833-9200.
- Worldwide, visit www.tektronix.com to find contacts in your area.

Kit description

This kit describes the installation of the Option 51 Preamp upgrade in the instruments listed below.

Products

RSA5115A. All serial numbers

RSA5126A. All serial numbers

Kit parts list

Quantity	Part number	Description
1 ea	071-3094-xx	MANUAL,TECH: INSTALLATION INSTRUCTIONS,RSA5UP OPT 51, RSA5115A/RSA5126A PREAMP UPGRADE
1 ea	NS ¹	LABEL, MANUFACTURED; OPTION KEY UPGRADE LABEL

¹ NS – Not saleable

Installation instructions

The software for Option 51 (Preamp upgrade) requires the installation of an option key to activate the software.

Installation of any new option requires that the latest version of instrument software be installed.

Update the instrument application software


1. Select **Help > About** from the RSA analyzer menu bar.
Note the version of your analyzer's software.
2. Use your Web browser to go to: www.tektronix.com/software.
3. Enter your instrument model number in the **Search by keyword** text box and click **Go**.

4. Follow the link for the analyzer software.
5. Note the version of the available software.
 - If your instrument's software matches the available version, no software update is necessary and proceed to installing the option key.
 - If your instrument's software is older than the available version, follow the instructions on the Web page to download and install the software before installing the option key.


Install option key

To activate the option:

1. In the analyzer application, select **Tools > Install Upgrades**. The Install Upgrade wizard will start. Click **Continue**.

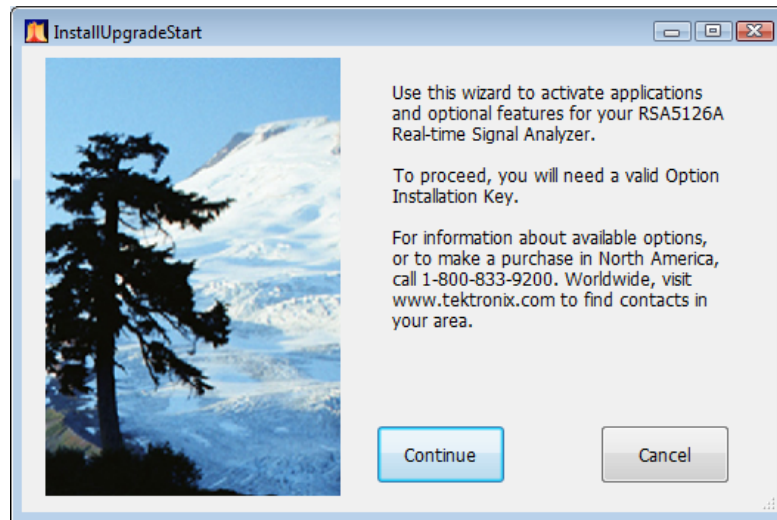

2. The Install Upgrade Enter Key screen appears.

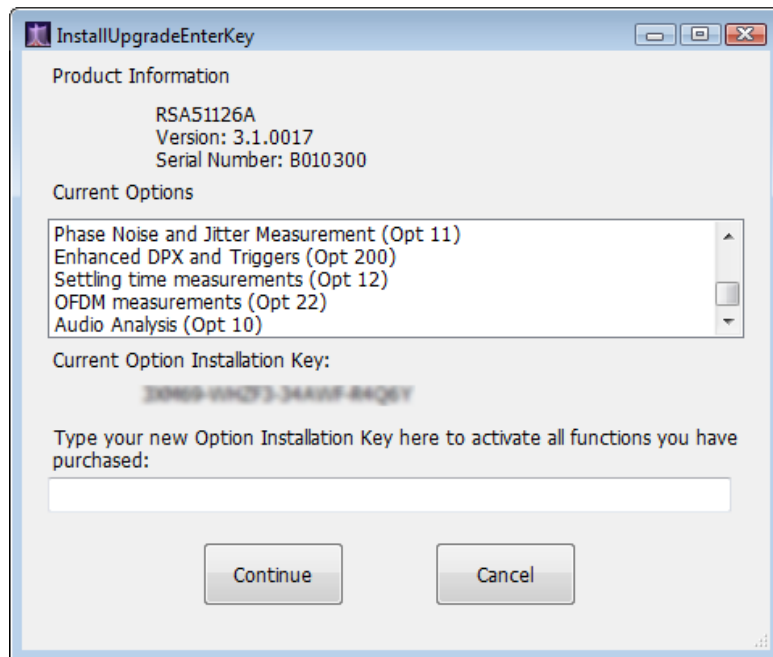

3. Type the option installation key into the empty text box and click **Continue**. An **Install Upgrade Success** dialog box opens.
4. Click **Close**. Exit and restart the analyzer application to enable the new feature.
5. In the Help menu, select About Tektronix Real-Time Analyzer.
6. Look in the **Installed Options** list and verify that **Internal Preamp (Opt 51)** appears.

Install label

1. Place the new option key label over the existing label on the instrument rear panel.

This completes the installation of the Option 51.

■ End of Document ■