

**SPECMONBUP (Software Options)  
SPECMONB Series Real-Time Spectrum Analyzers  
Software Only Upgrades**

**Instructions**

[www.tektronix.com](http://www.tektronix.com)



075-1067-00

**Tektronix**

Copyright © Tektronix. All rights reserved. Licensed software products are owned by Tektronix or its subsidiaries or suppliers, and are protected by national copyright laws and international treaty provisions.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specifications and price change privileges reserved.

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

---

## Kit description

This kit provides instructions to activate software upgrades to the SPECMONB Series Real-Time Signal Analyzers.

The option you've ordered only requires that you enter a key code to activate your option.

For a list of available options, see the Tektronix Web site ([www.tektronix.com](http://www.tektronix.com)) or your Tektronix representative.

## Products

**SPECMON3B.** All serial numbers

**SPECMON6B.** All serial numbers

**SPECMON26B.** All serial numbers

## Option kit parts list

Quantity	Part number	Description
1 ea	075-1067-xx	INSTRUCTIONS, UPGRADE: SPECMONBUP SOFTWARE OPTIONS
1 ea	N/A	LABEL, MANUFACTURED; OPTION KEY UPGRADE LABEL 2.100 X 2.700, SAFETY CONTROLLED
1 ea	N/A	LABEL, MANUFACTURED; PRODUCT LABEL, SAFETY CONTROLLED <b>NOTE.</b> Not included with all options.
1 ea	N/A	LABEL, EXPORT CONTROL CLASSIFICATION <b>NOTE.</b> The Export Control label is only included with Options 09, 65, or 6566.


## Minimum tool and equipment list

Name	Description
Keyboard	Standard accessory provided with the instrument


## Install option key

To activate your new option, you must enter a new option key.

1. Power on the instrument.
2. Select **Tools > Install Upgrades...** to start the upgrade installation process.
3. Click Continue from the Install Upgrades introduction screen.

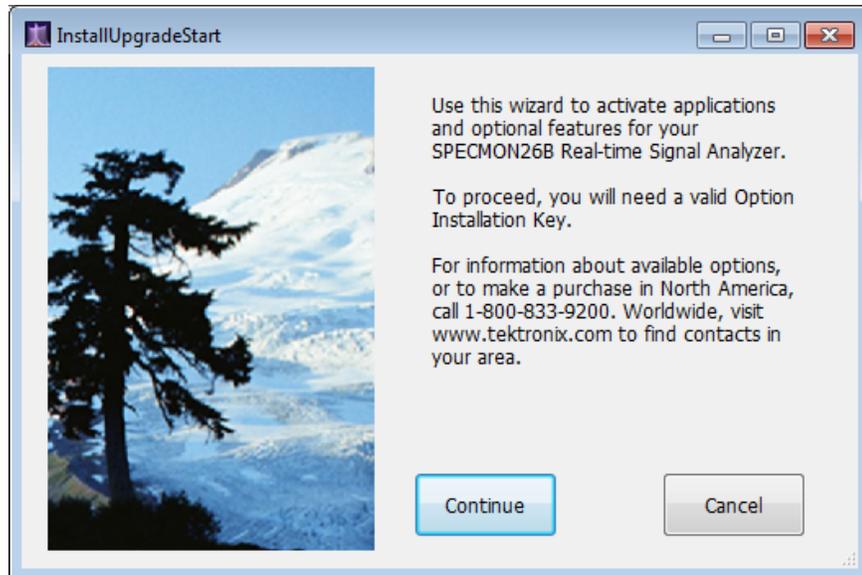

4. Enter the option key provided by Tektronix, and follow the on-screen instructions to install the option.

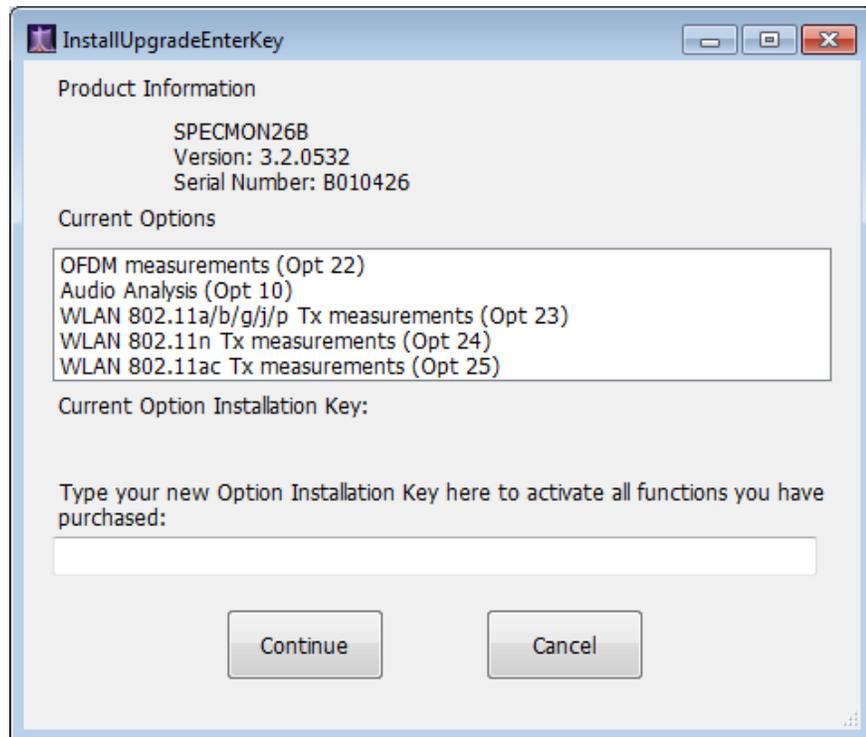

5. Power off the instrument, then power back on.
6. In the Help menu, select About Tektronix Real-Time Analyzer.
7. Verify the new option is listed.

## Attach labels

Please attach all labels provided in this kit on the instrument's rear panel.

**Attach the option key label** Place the new option key label over the existing label on the instrument rear panel.

---

**NOTE.** *This label is not included with all options.*

---

**Attach the product/option label** Place the new product key label over the existing label on the instrument rear panel if this label is included with your option.

**Attach the Export Control classification label** Place the Export Control classification label on the instrument rear panel.

---

**NOTE.** *The Export Control label applies only to the SPECMONB Series instruments when installing Options 09, 65, or 6566.*

---

## Verify instrument software version

Tektronix recommends to update to the latest available application software for your instrument.

1. Select **Help > About** to check the software version.
2. Use your Web browser to go to: [www.tektronix.com/software](http://www.tektronix.com/software).
3. Search for your instrument's model number and follow the link to the software.
4. If the installed software is older than that available, download the software.
5. Follow the instructions on the Web page to install the software.

■ End of Document ■